


The background is a light gray gradient. It is decorated with several realistic water droplets of various sizes, some at the top and some at the bottom. In the upper center, there is a faint, circular logo or watermark that appears to be a university crest.

KERATOGRAF


ZDRAVKO BELJAN MSC. OPT.

ZAGREB, 25. STUDENI 2017.

KERATOGRAF

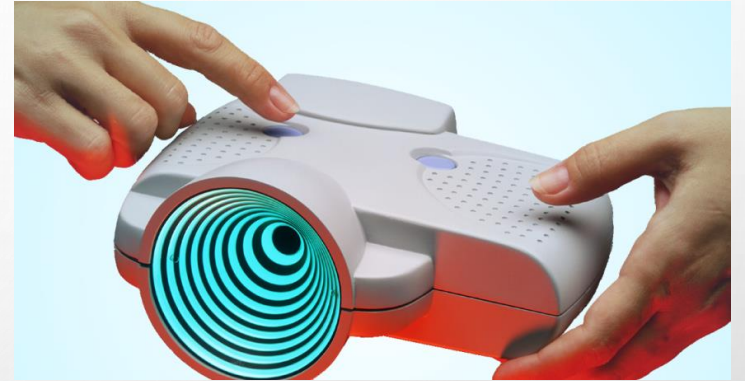

KERATOGRAPH

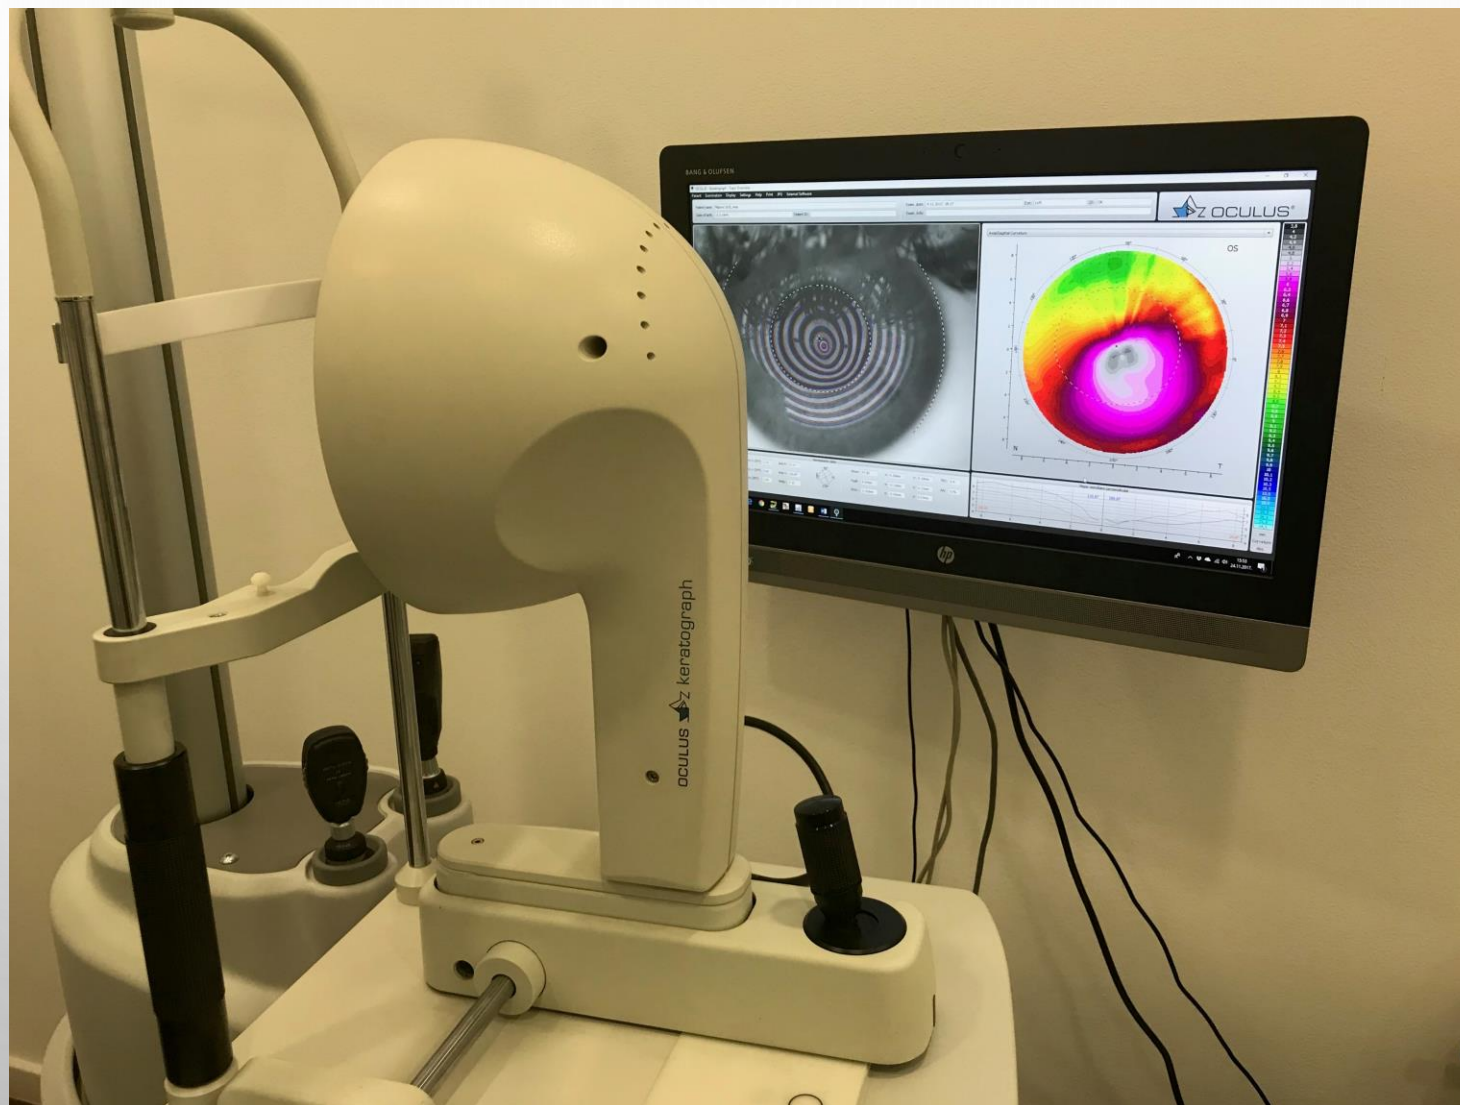

KERATOGRAF

- Zlatni standard današnjeg mjerenja kornealne površine
- Osigurava razumijevanje oblika te analizu površine rožnice
- Preciznost instrumenta osigurava reproduktibilnost mjerenja
- Softver instrumenta konzultira u odabiru kontaktnih leća i virtualnim fitanjem odabire najbolju moguću leću
- Program "Analiza suznog filma" daje opširan prikaz stabilnosti suznog filma u realnom vremenu te prikaz i mjere suznog meniska
- Noviji modeli instrumenta omogućavaju meibomografiju
- Omogućeno je povezivanje na vanjske programe proizvođača kontaktnih leća

KERATOGRAM

- Uz pomoć keratografa može se razumjeti neka neuobičajena stanja u refrakciji

KERATOGRAF

SLUČAJ MONOKULARNE DIPLOPIJE

Pacijent

KUMP TINA
ZVONIMIROVA 94
10000 ZAGREB
Prezime i ime (naziv)
Id:

HZZO Kartoteka Potvrdi unos

Zdravnik: 01
Saznali za nas:
Status: Reklamacija ☐

Napomena na dokumentu
Bolesti oka i adneksa

Dioptrija naočala i leća Keratometrija

Dioptrija daljina

	Sph	CYL	AXE	ADD	Prizma	Smjer	Dec
D	-0,25	-0,25	172	0,00	0,00	0	0
	-0,50	+0,25	82				
L	+0,00	-0,25	20	0,00	0,00	0	0
	-0,25	+0,25	110				

PD 0,0 0,0
Potvrdi


VSC DO 0,6
LO 0,8(-)
VCC DO 0,8(-)
LO 1,00

Dioptrija blizina

Žali se na dvoslike
monokularno


S refrakcijom ne
postizem nestanak
dvoslike

KERATOGRAM

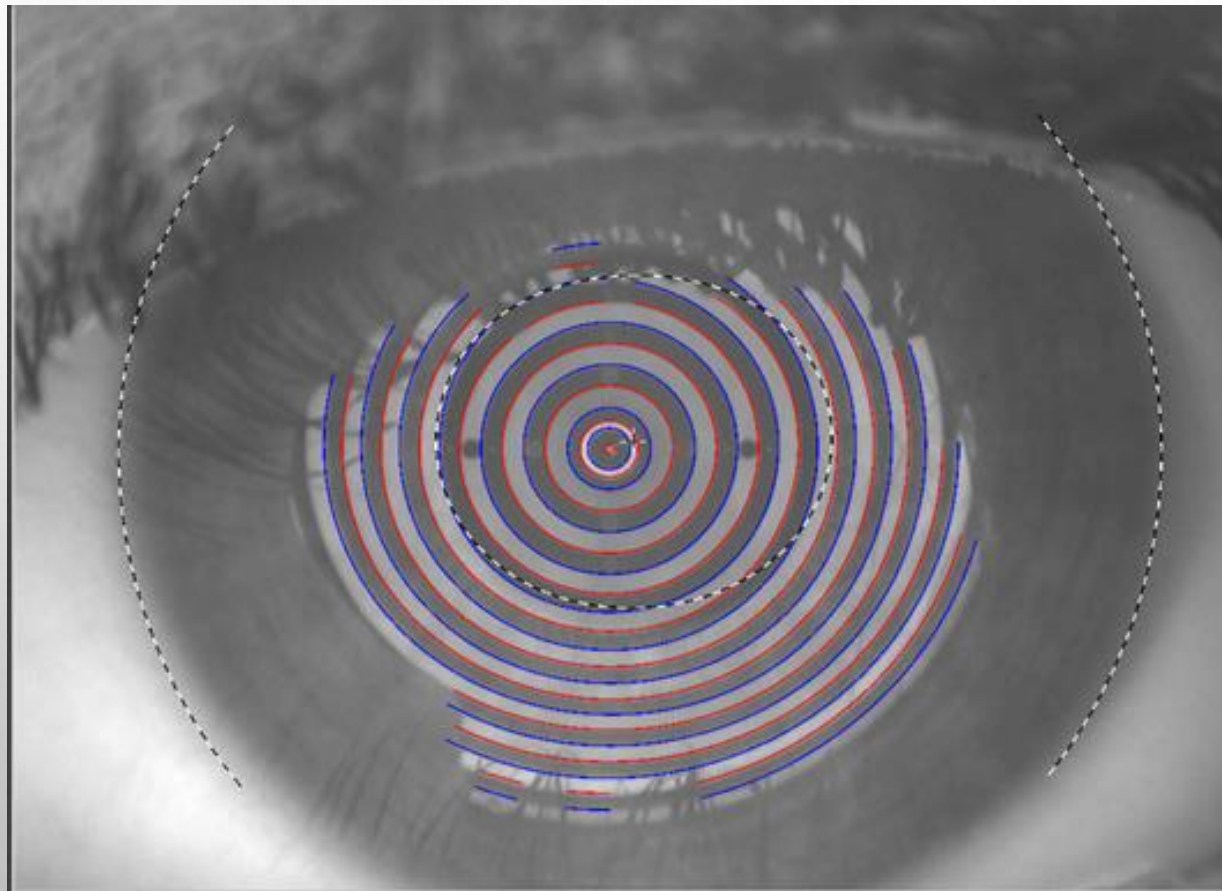


Rh: 7.66mm	K1: 44.10	ecc.h.(30°): 0.55	Axis h: 174.1°
Rv: 7.55mm	K2: 44.70	ecc.v.(30°): 0.16	Axis v: 84.1°
Rm: 7.60mm	Km: 44.40	ecc.(30°): 0.35	Astg.: -0.6D

Kmax: 46.00	x: -0.20mm	y: -3.10mm	TKC: -
Pupil: 4.29mm	x: 0.29mm	y: 0.08mm	AA: 56%
Decor: 12.29mm	x: 0.37mm	y: -0.03mm	

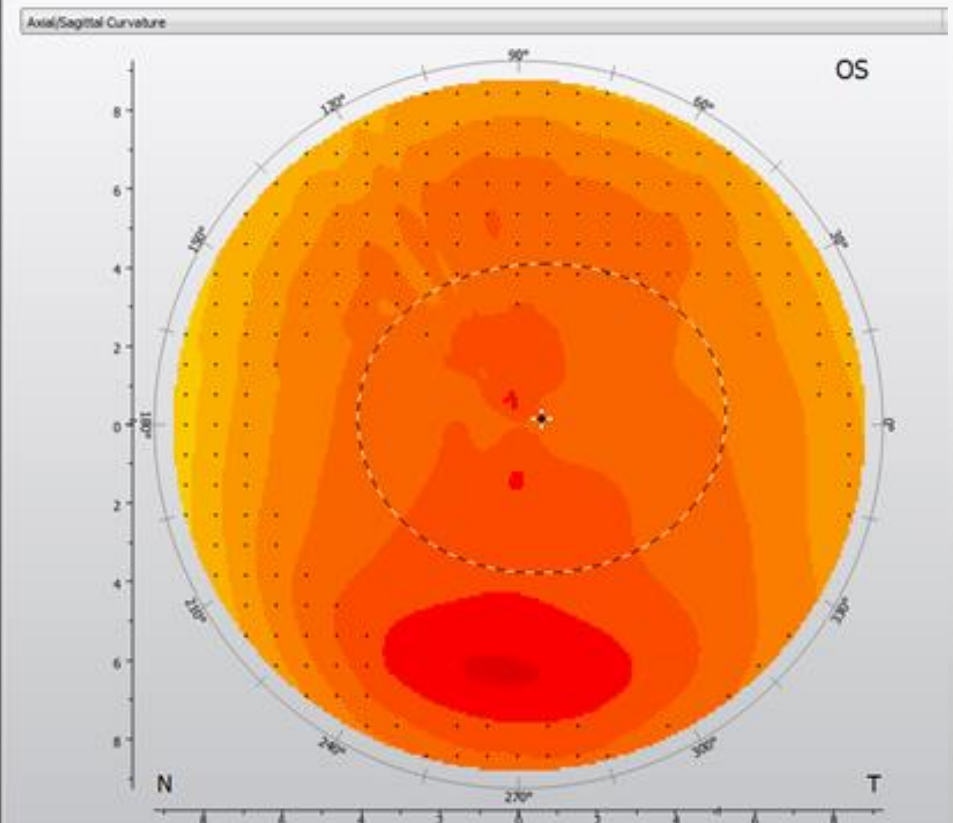


KERATOGRAF

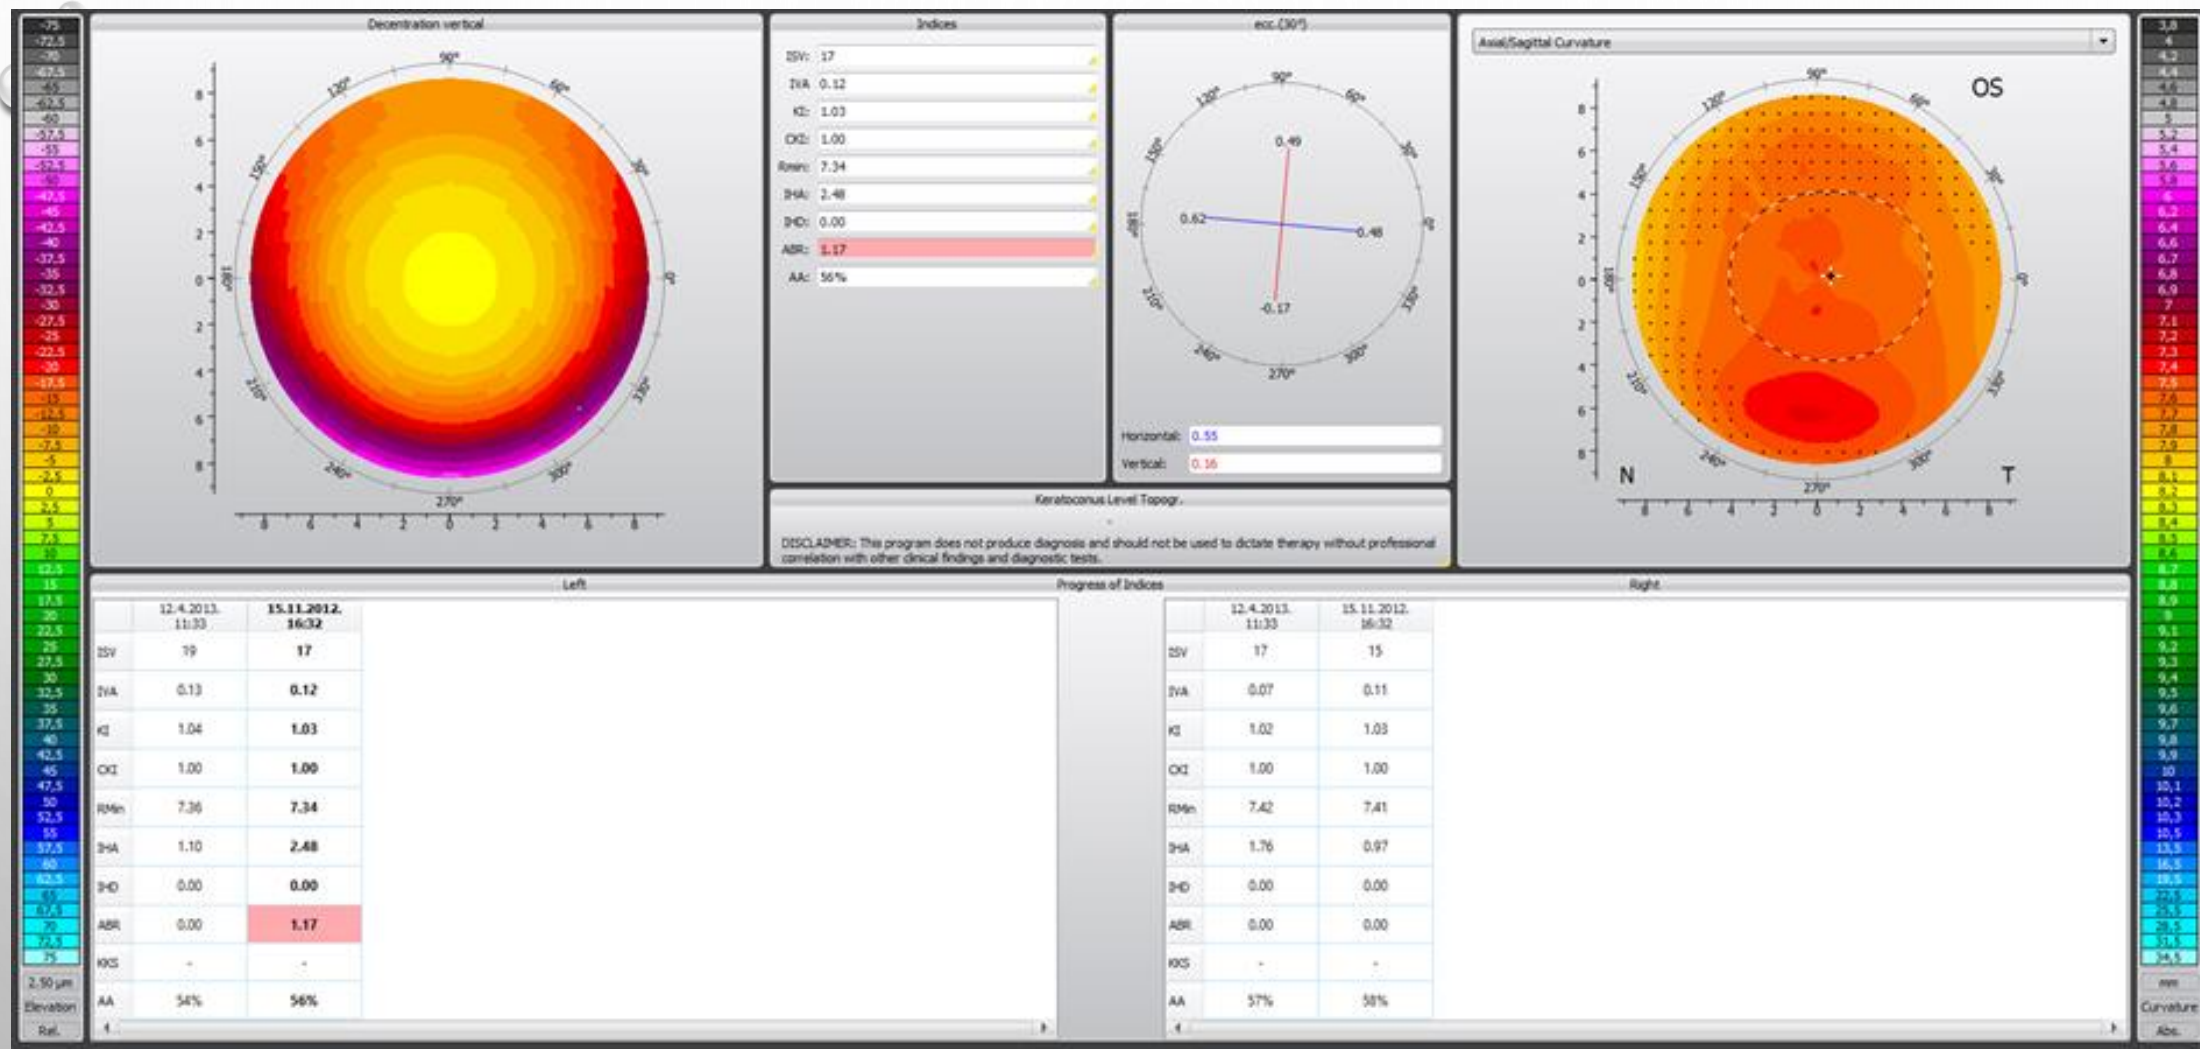

- Topografija ne ukazuje na veće iregularnosti rožnice

KERATOGRAF

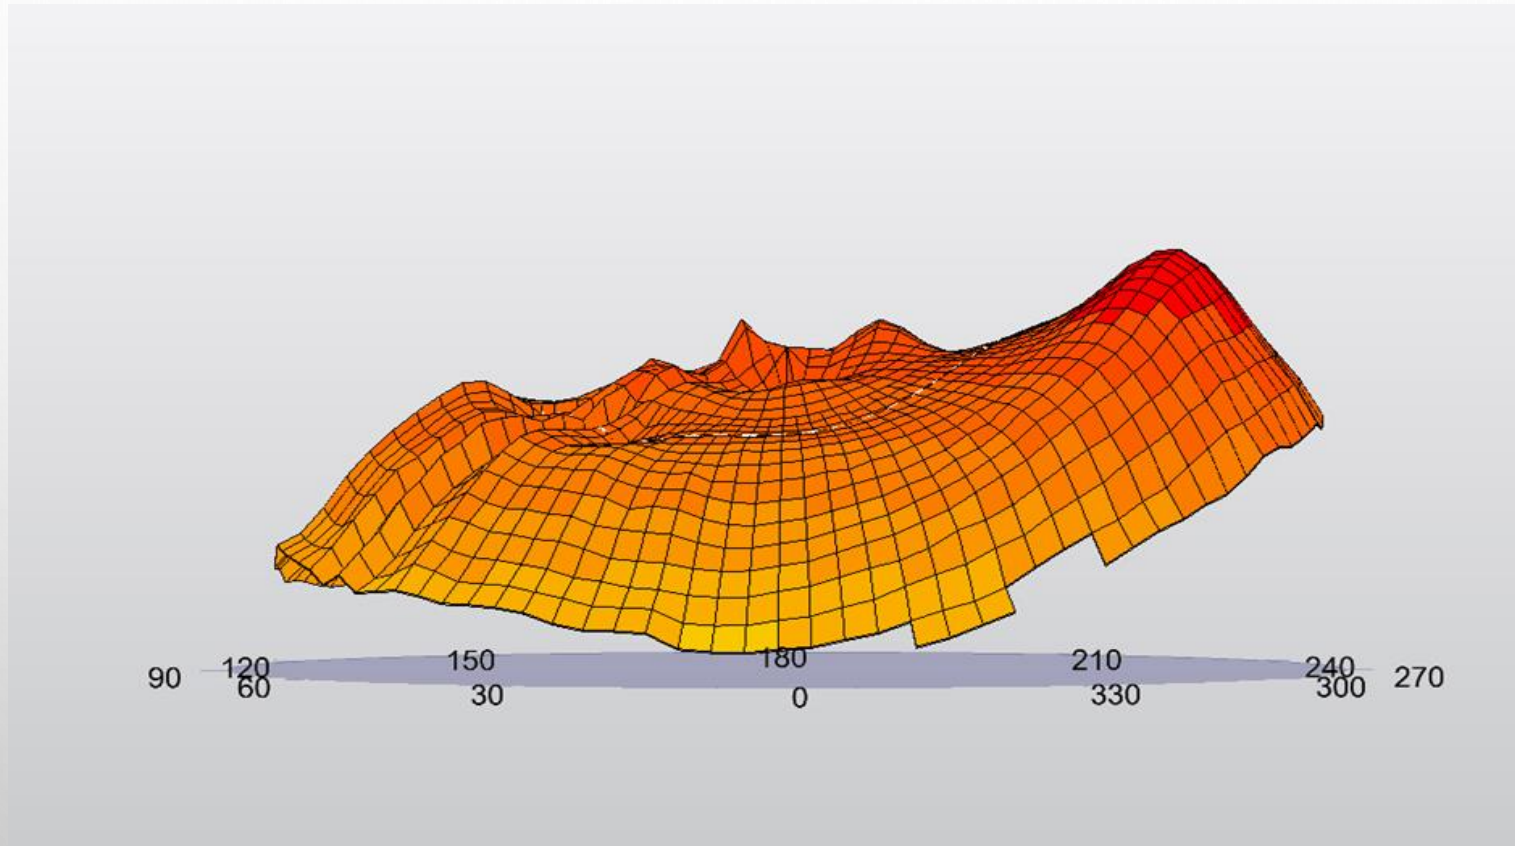

- Tek karikirana simulacija topografije rožnice otkriva mogući uzrok monokularne duplopije

KERATOGRAM

Pacijent
KUMP TINA
ZVONIMIROVA 94
10000 ZAGREB

HZZO Kartoteka Potvrdi unos Ispis POS E8 Kartica Ispis A4 E9

Zdravnik: 01
Saznali za nas:
Status: Reklamacija

Napomena na dokumentu:
Bolesti oka i adneksa

Dioptrija naočala i leća Keratometrija

Dioptrija daljina

	Sph	CYL	AXE	ADD	Prizma	Smjer	Dec
D	-0,25	-0,25	172	0,00	0,00	0	0
	-0,50	+0,25	82				
L	+0,00	-0,25	20	0,00	0,00	0	0
	-0,25	+0,25	110				

PD 0,0 0,0 Potvrdi

VSC DO 0,6
LO 0,8(-)
VCC DO 0,8(-)
LO 1,00

Dioptrija blizina

D	+0,00	+0,00	0	0,00	0,00	0	0
L	+0,00	+0,00	0	0,00	0,00	0	0

0,0 0,0 Potvrdi

Dioptrija računalo

D	+0,00	+0,00	0	0,00	0,00	0	0
L	+0,00	+0,00	0	0,00	0,00	0	0

0,0 0,0 Potvrdi

Kontaktne leće

	B.C.	Dia	Sph	CYL	AXE	Visus
D	7,80	10,00	-0,50	+0,00	0	1,00
L	7,70	10,00	-0,50	+0,00	0	1,00

Potvrdi

Opto centar comf. optimum comfort , bl, dot

- Kontaktna leća uklanja monokularnu duplopiju

SLUČAJ MONOKULARNE DIPLOPIJE 2

Pacijent	HZZO	Kartoteka	Potvrdi unos
DELBONO GIUSEPPE	Zdravnik:	Napomena na dokumentu	
	01	VISUS D.O./L.O 0,4/0,8	
compagnladeebono@emilianomagnateato.com	Saznali za nas:	D.O. KK1	
		L.O. ABER	
	Status	Bolesti oka i adneksa	
	Reklamacija		


Dioptrijska daljina		Keratometrija					
	Sph	CYL	AXE	ADD	Prizma	Smjer	Dec
D	+0,50	-0,75	170	0,00	0,00	0	0
	-0,25	+0,75	80				
L	+0,25	-0,50	15	0,00	0,00	0	0
	-0,25	+0,50	105				

Dioptrijska blizina	
D	+0,00 +0,00 0 0,00 0,00 0 0
L	+0,00 +0,00 0 0,00 0,00 0 0


Dioptrijsko računalno	
D	+0,00 +0,00 0 0,00 0,00 0 0
L	+0,00 +0,00 0 0,00 0,00 0 0

Kontaktne leće					
B.C.	Dia	Sph	CYL	AXE	Visus
D	0,00	0,00	+0,00	+0,00	0 0,00
L	0,00	0,00	+0,00	+0,00	0 0,00

KERATOGRAM

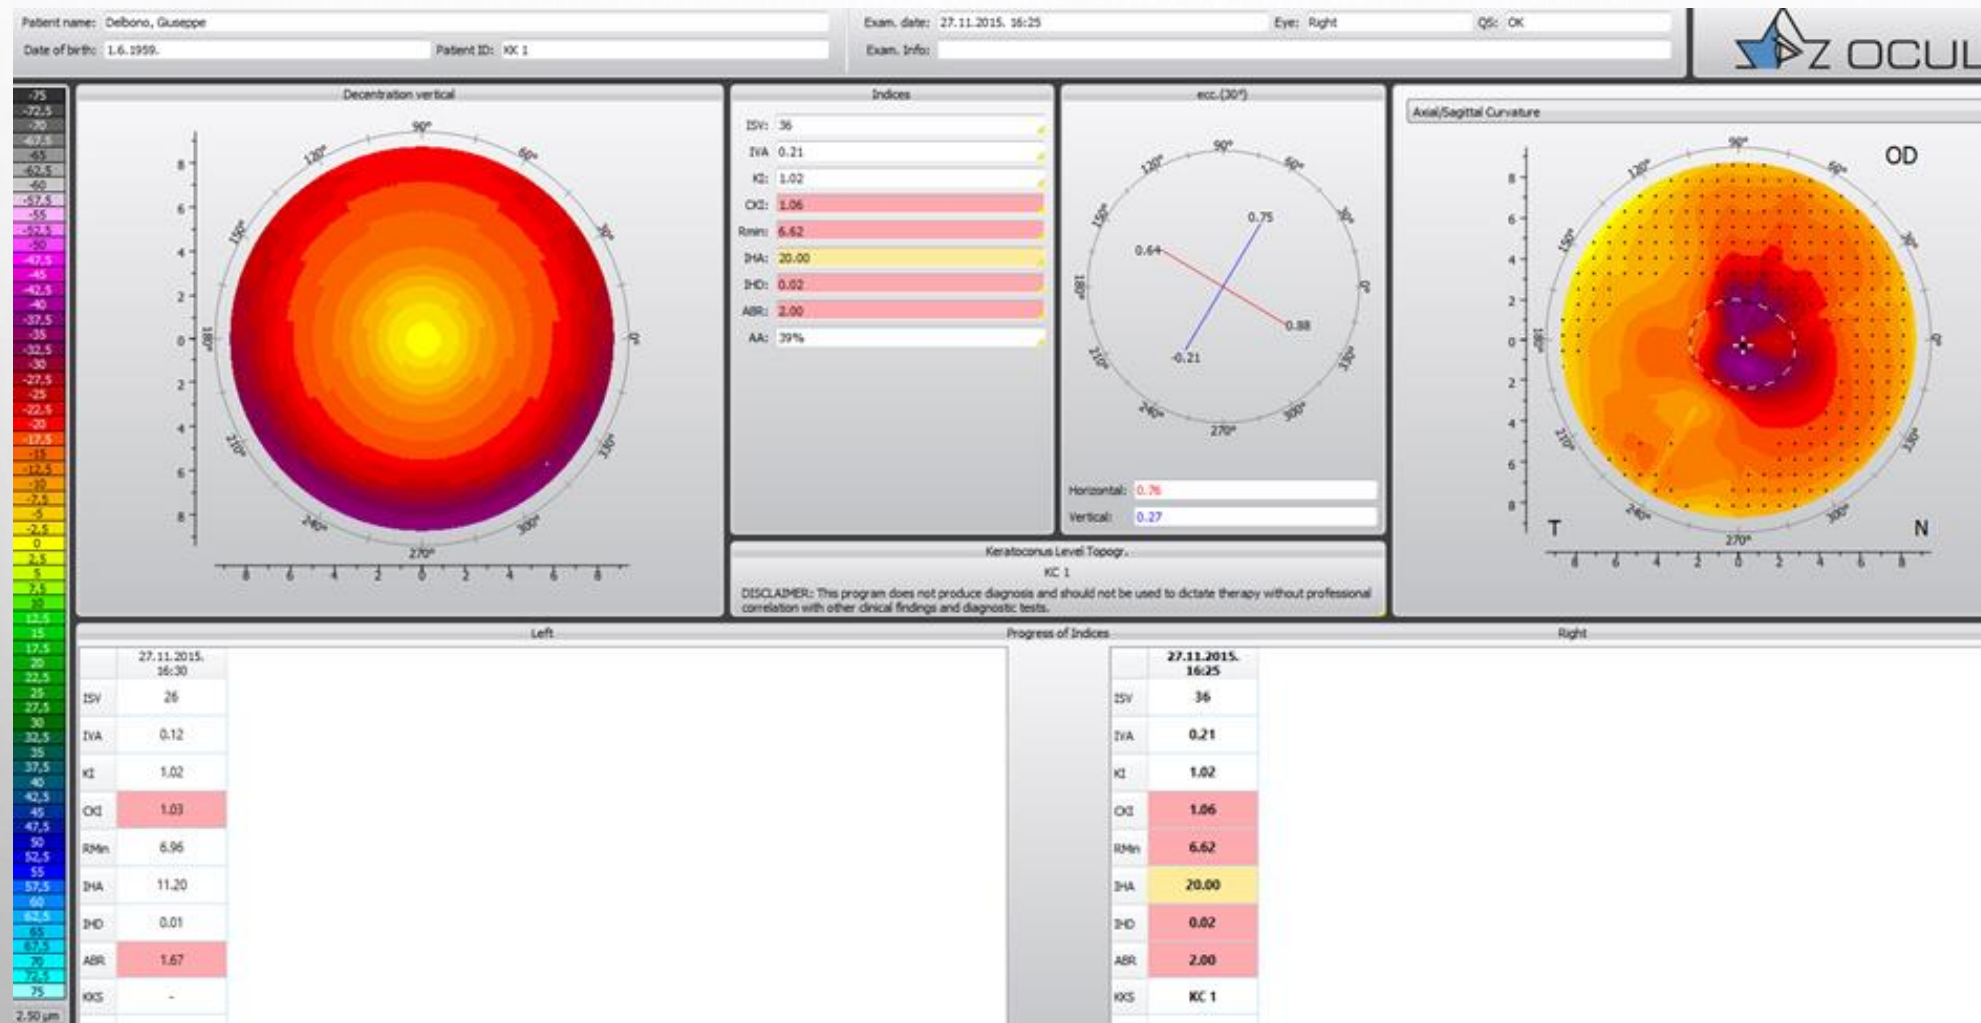


KERATOGRAM

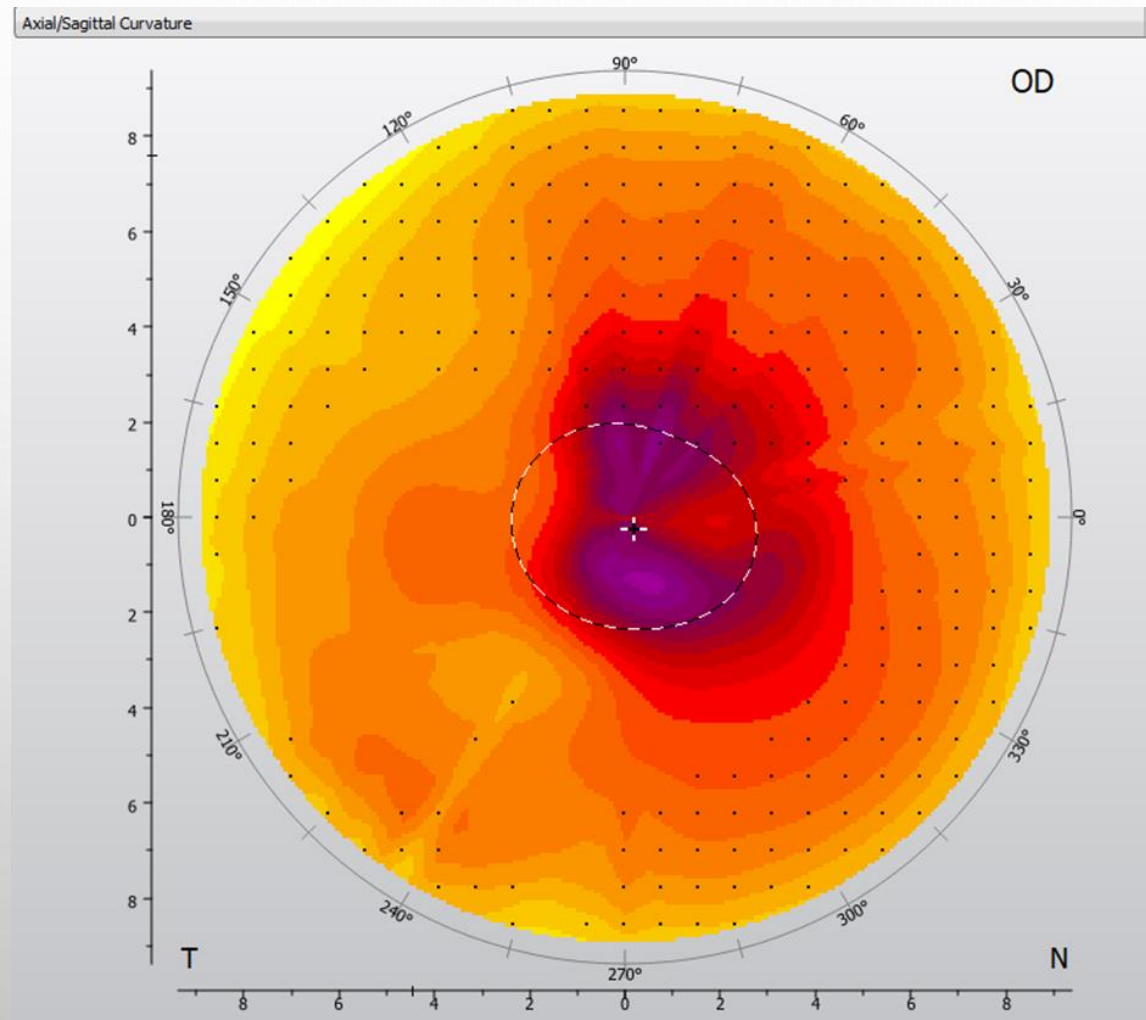


KK 1 nipple kone type

KERATOGRAM

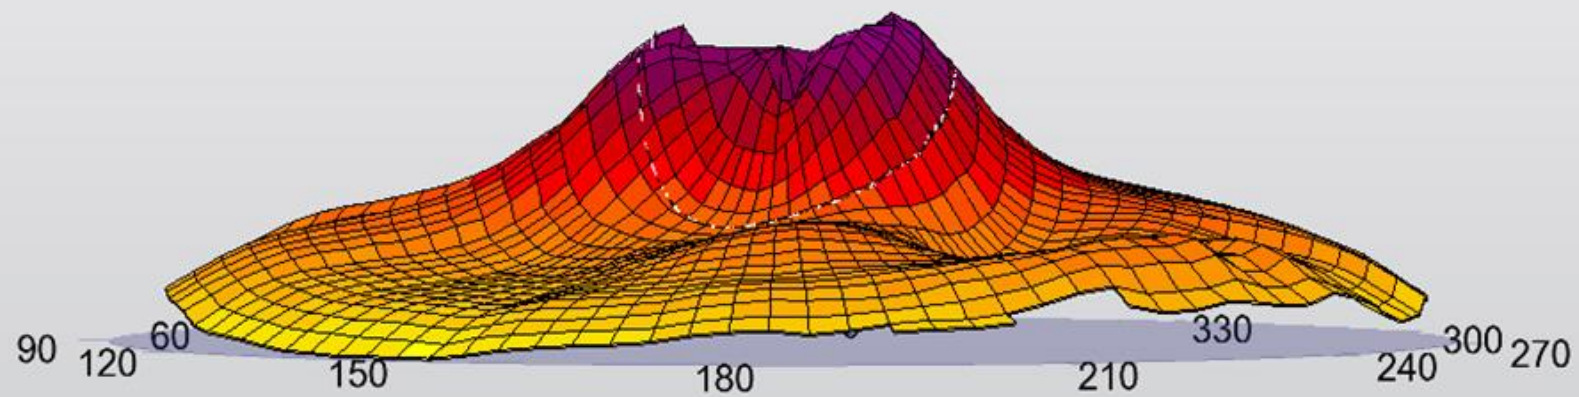

KERATOGRAM

SLUČAJ LUTAJUĆEG ASTIGMATIZMA

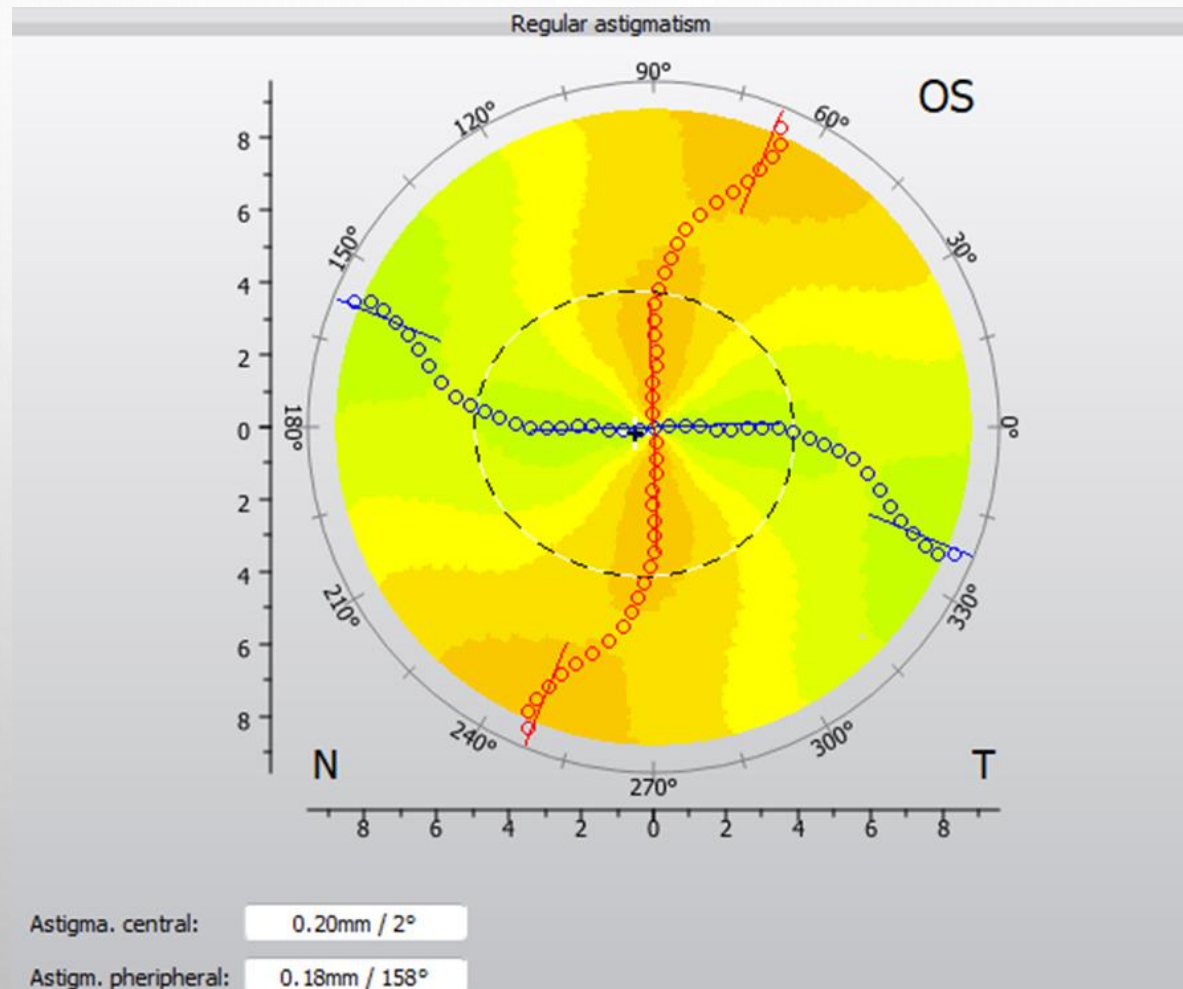

KERATOGRAF

SLUČAJ EKTAZIJA

Pacijent

KOVAČ Ph.D. IVAN

LUDINSKA 14

10000 ZAGREB

098211114

M

Id:

HZZO

Kartoteka

Potvrdi unos

Ispis POS E8

Ka

Zdravnik:

01

Saznali za nas:

Status

Reklamacija

Napomena na dokumentu

Bolesti oka i adneksa

Dioptrijska naočala i leća

Keratometrija

Dioptrijska daljina

	Sph	CYL	AXE	ADD	Prizma	Smjer	Dec
D	+0,00	-0,75	85	1,75	0,00	0	0
	-0,75	+0,75	175				
L	+0,50	-0,25	165	1,75	0,00	0	0
	+0,25	+0,25	75				

PD

33,0 33,0

Potvrdi

VISUS 1,25

Dioptrijska blizina

D	+0,00	+0,00	0	0,00	0,00	0	0
L	+0,00	+0,00	0	0,00	0,00	0	0

0,0 0,0

Potvrdi

Dioptrijska računalno

D	+0,00	+0,00	0	0,00	0,00	0	0
L	+0,00	+0,00	0	0,00	0,00	0	0

0,0 0,0


Potvrdi

Kontaktne leće


	B.C.	Dia	Sph	CYL	AXE	Visus
D	0,00	0,00	+0,00	+0,00	0	0,00
L	0,00	0,00	+0,00	+0,00	0	0,00

Potvrdi


KERATOGRAM

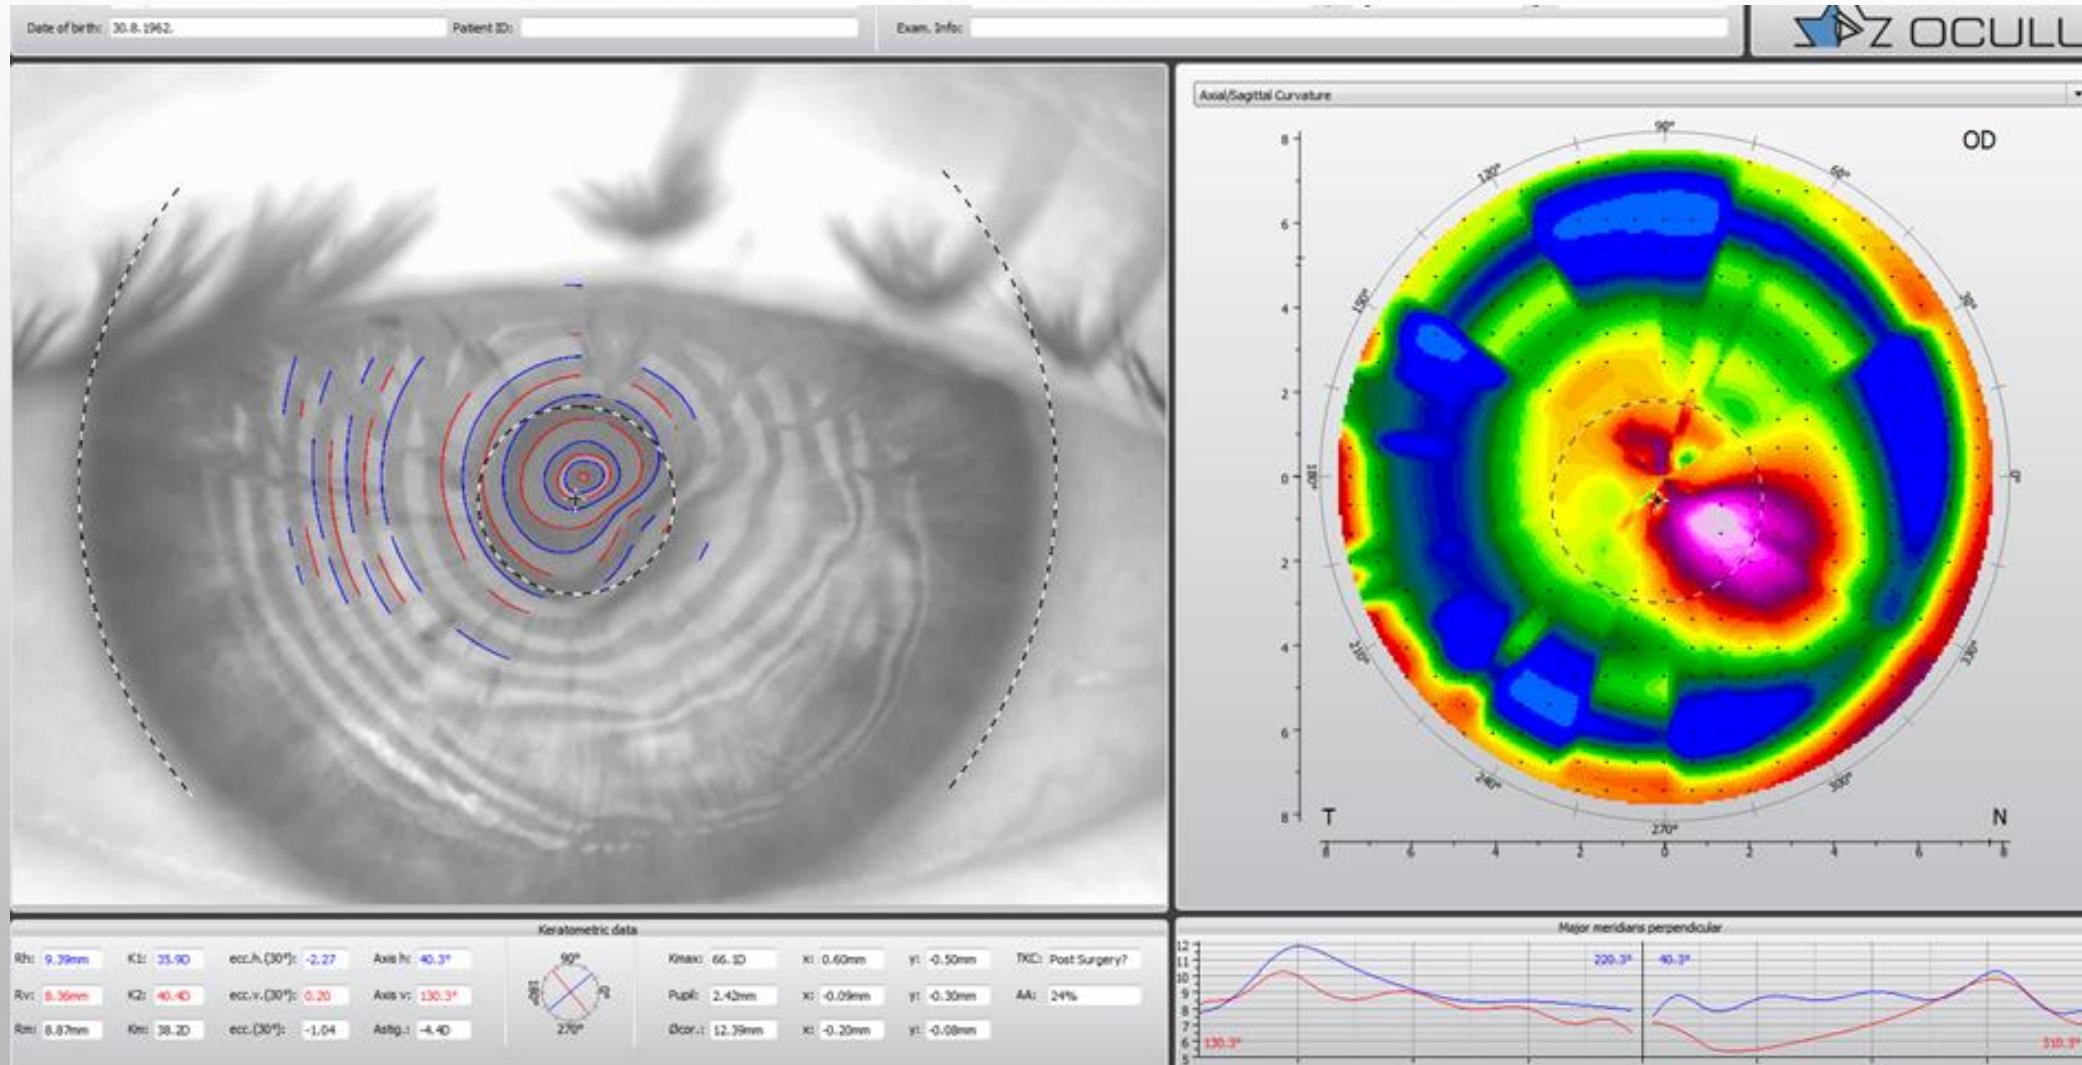

KERATOGRAM

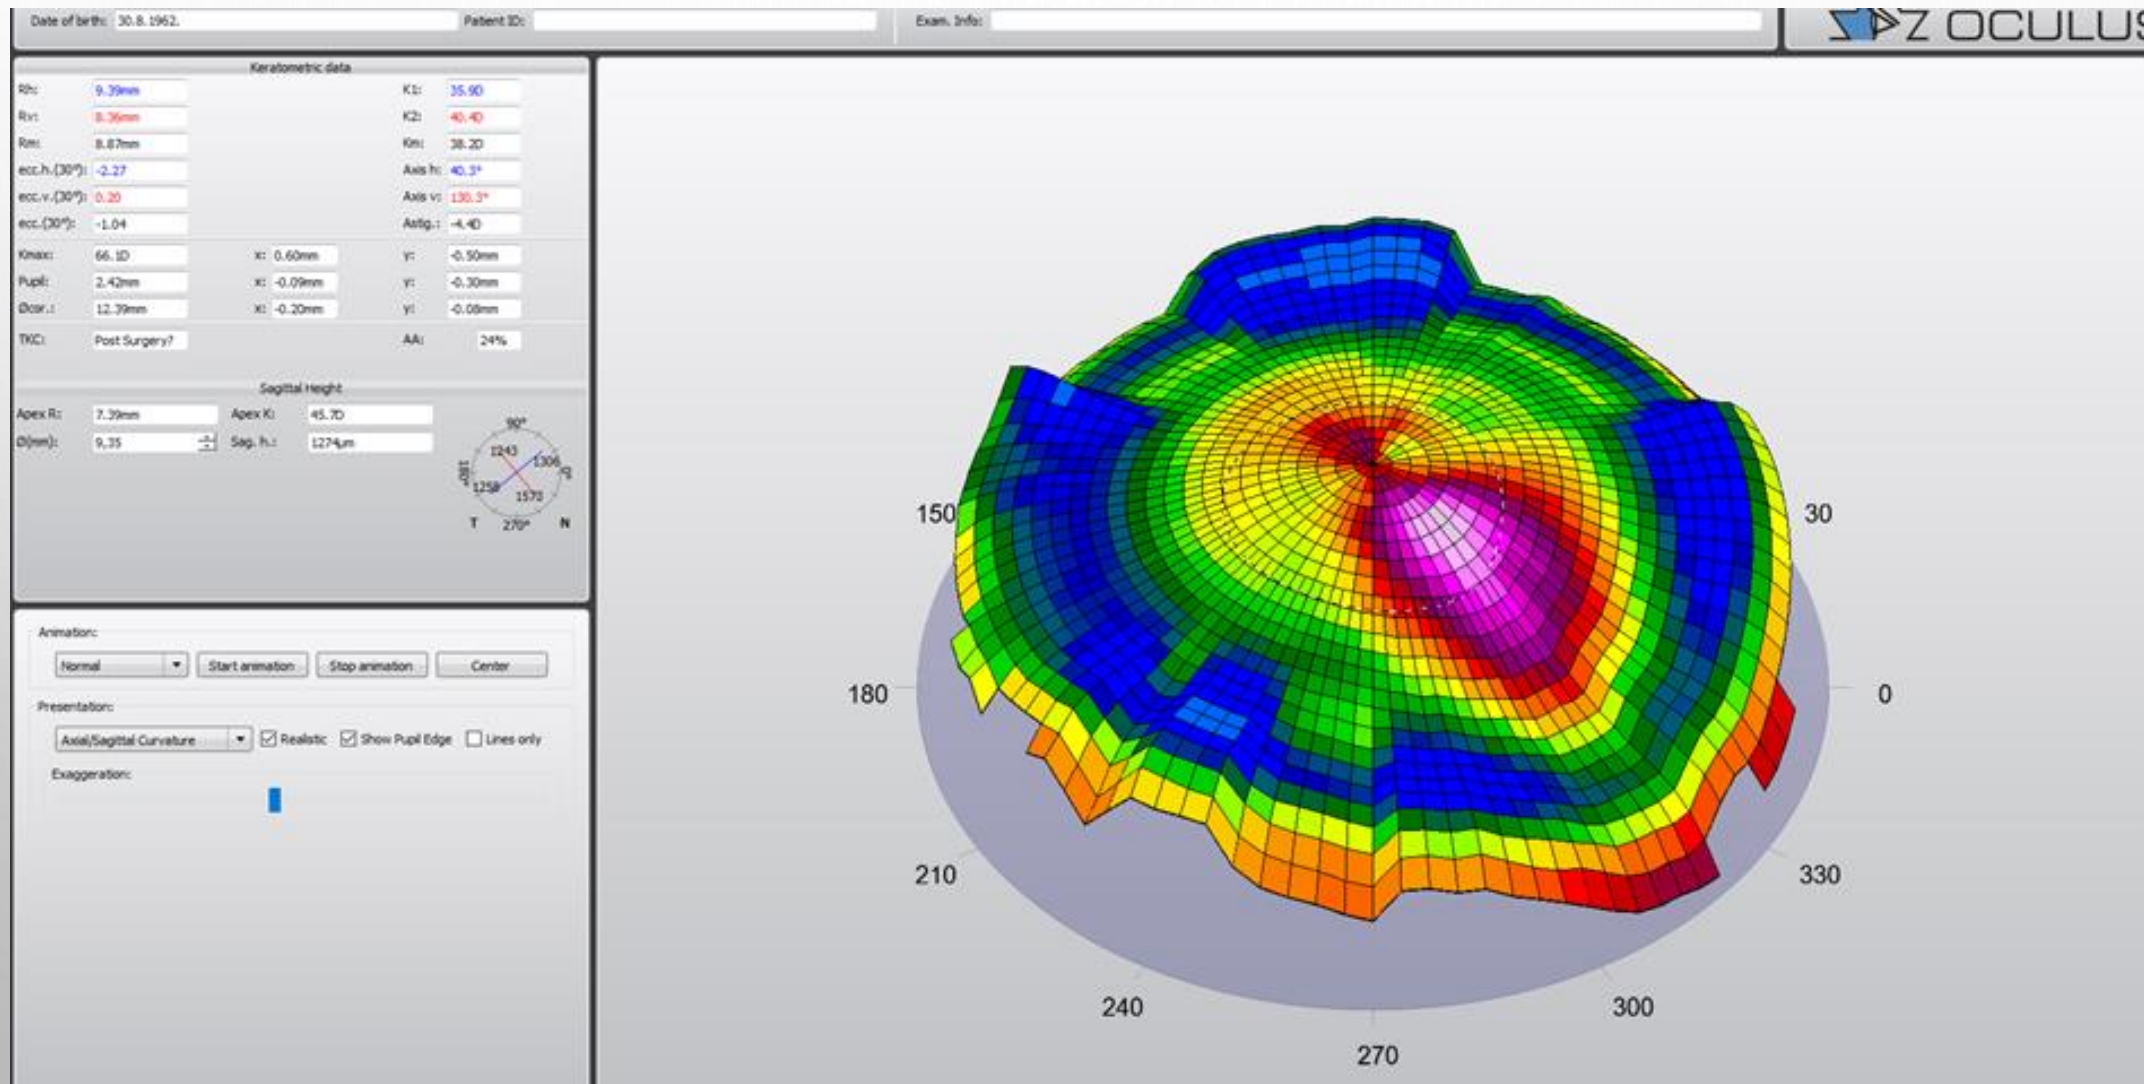

KERATOGRAM

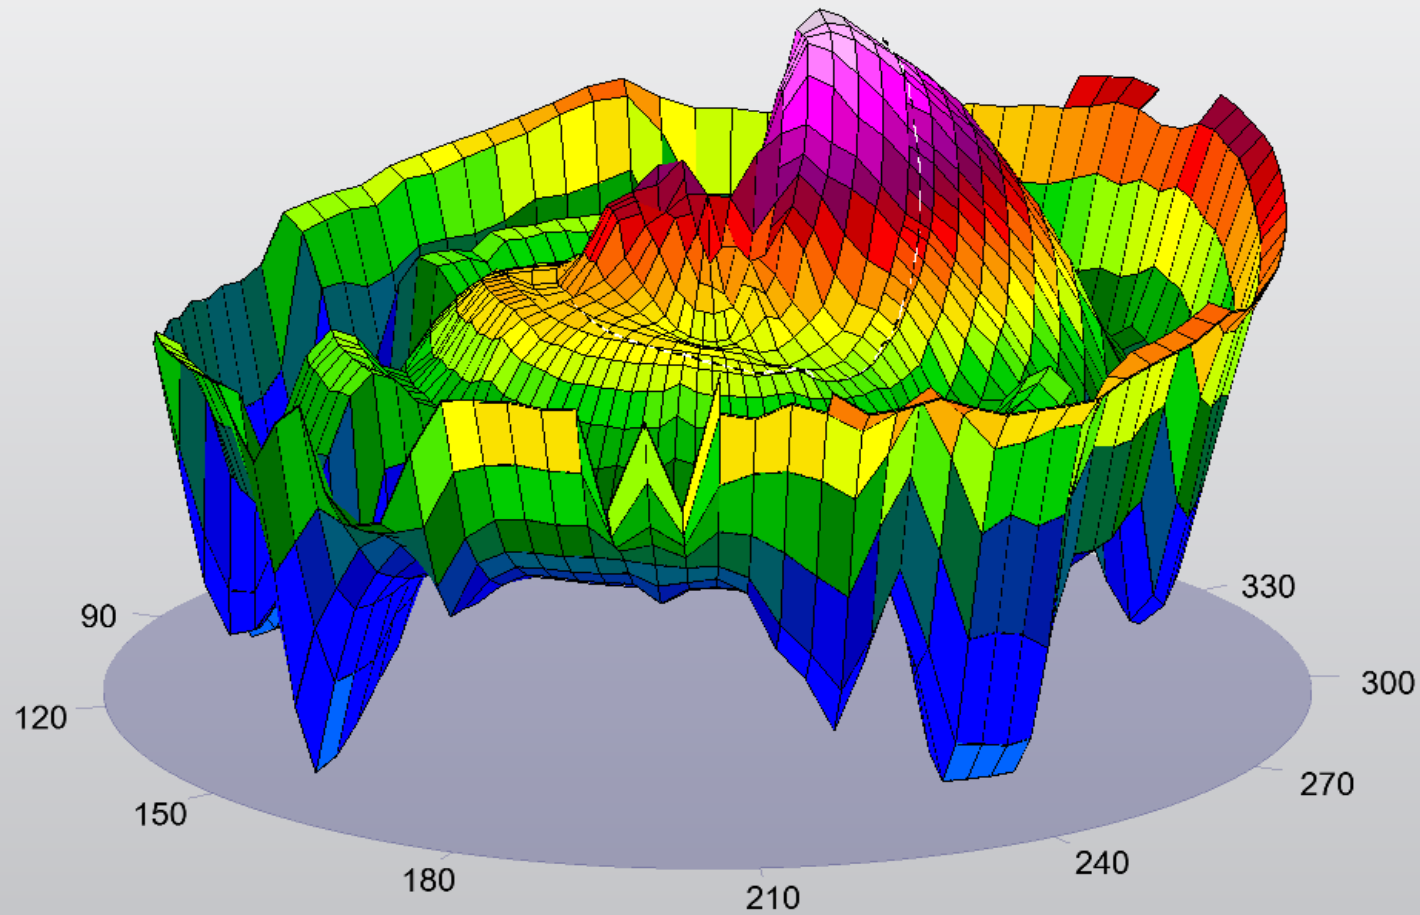




KERATOGRAF

ANALIZA SUZNOG FILMA




KERATOGRAF

SUZNI MENISKUS

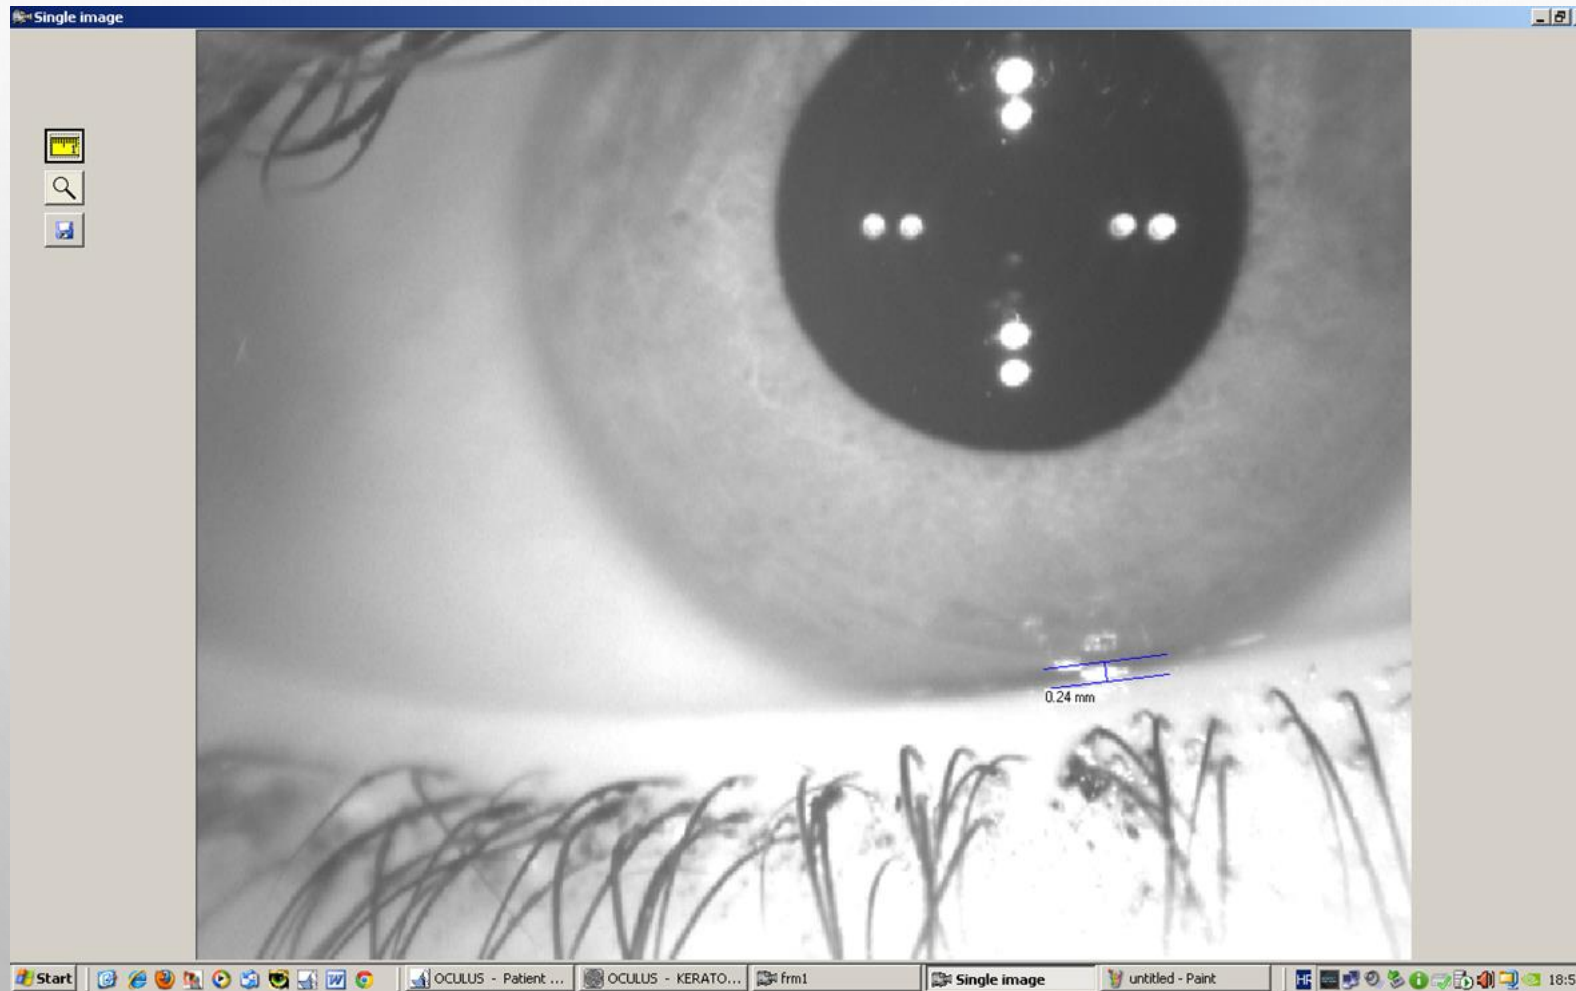


KERATOGRAM


NIK BUT

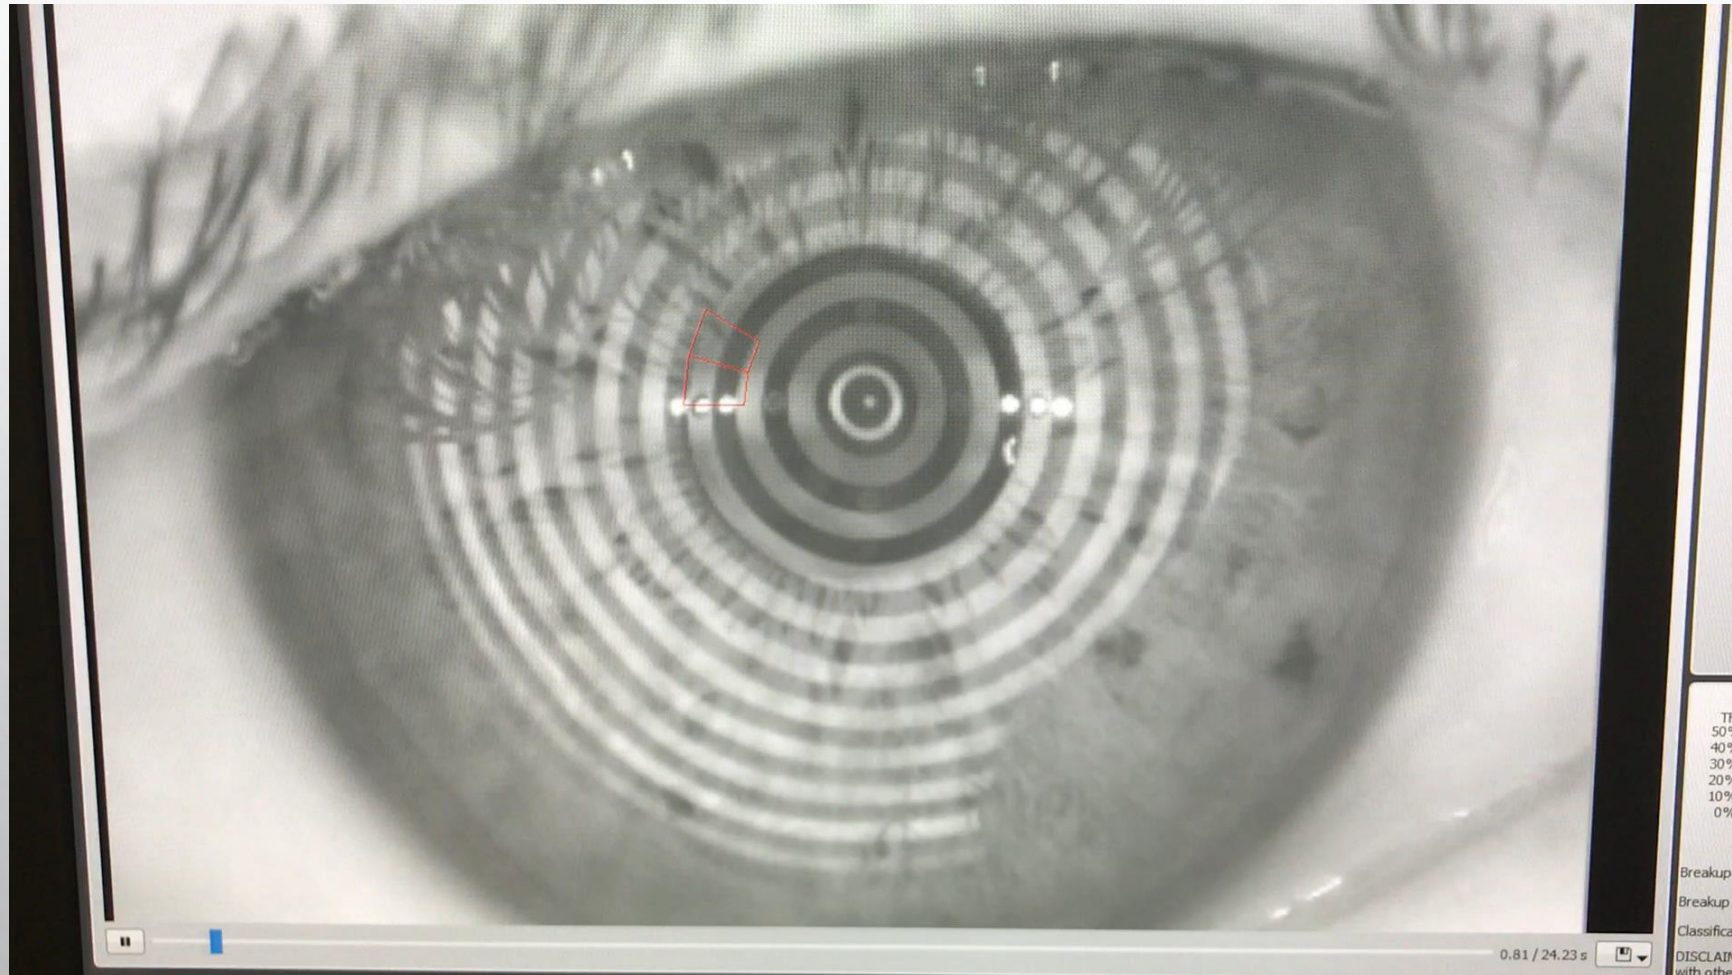

KERATOGRAM

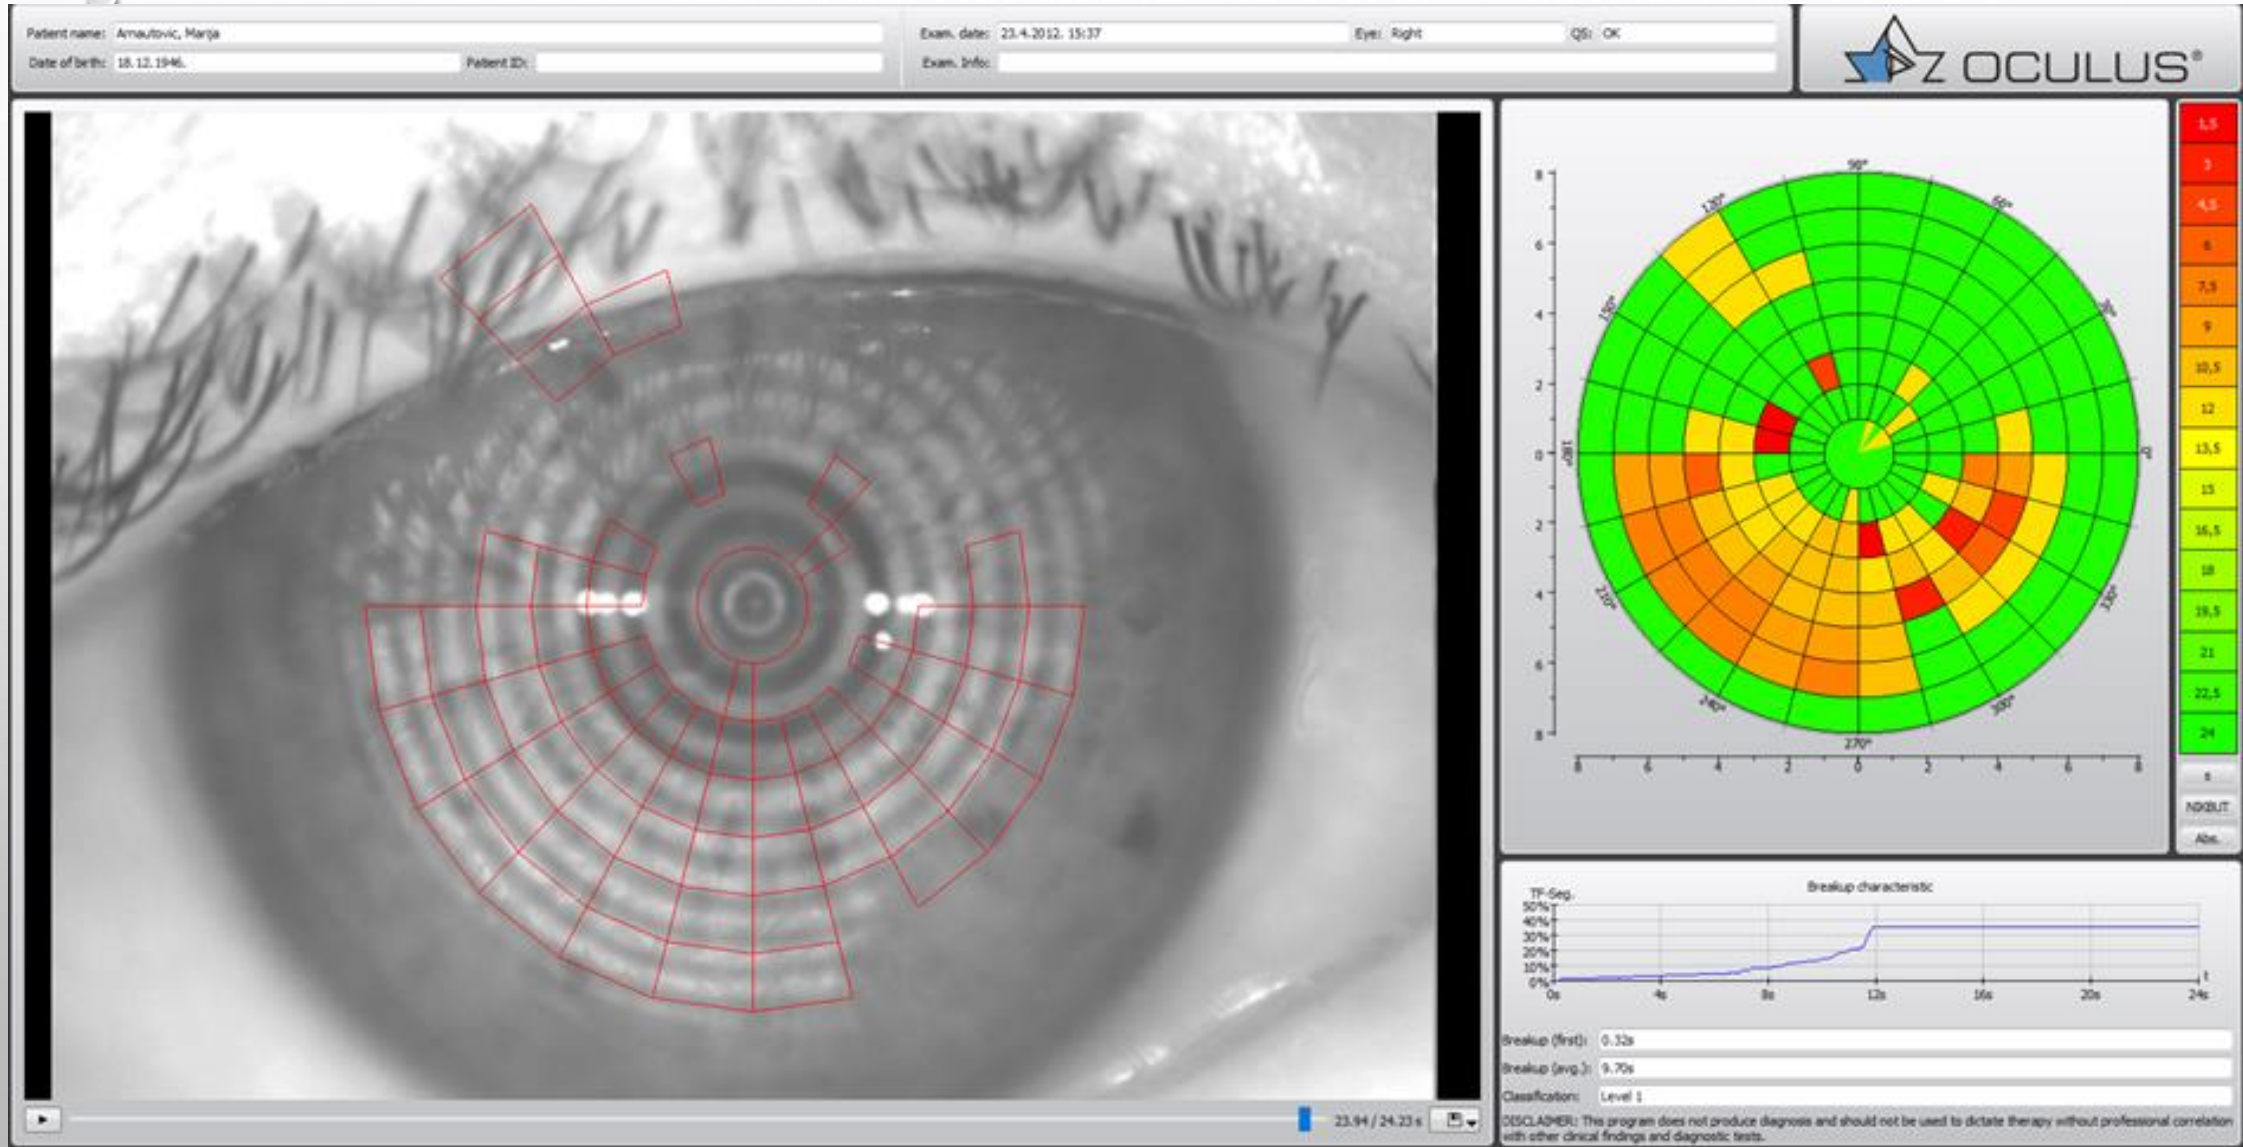


KERATOGRAM

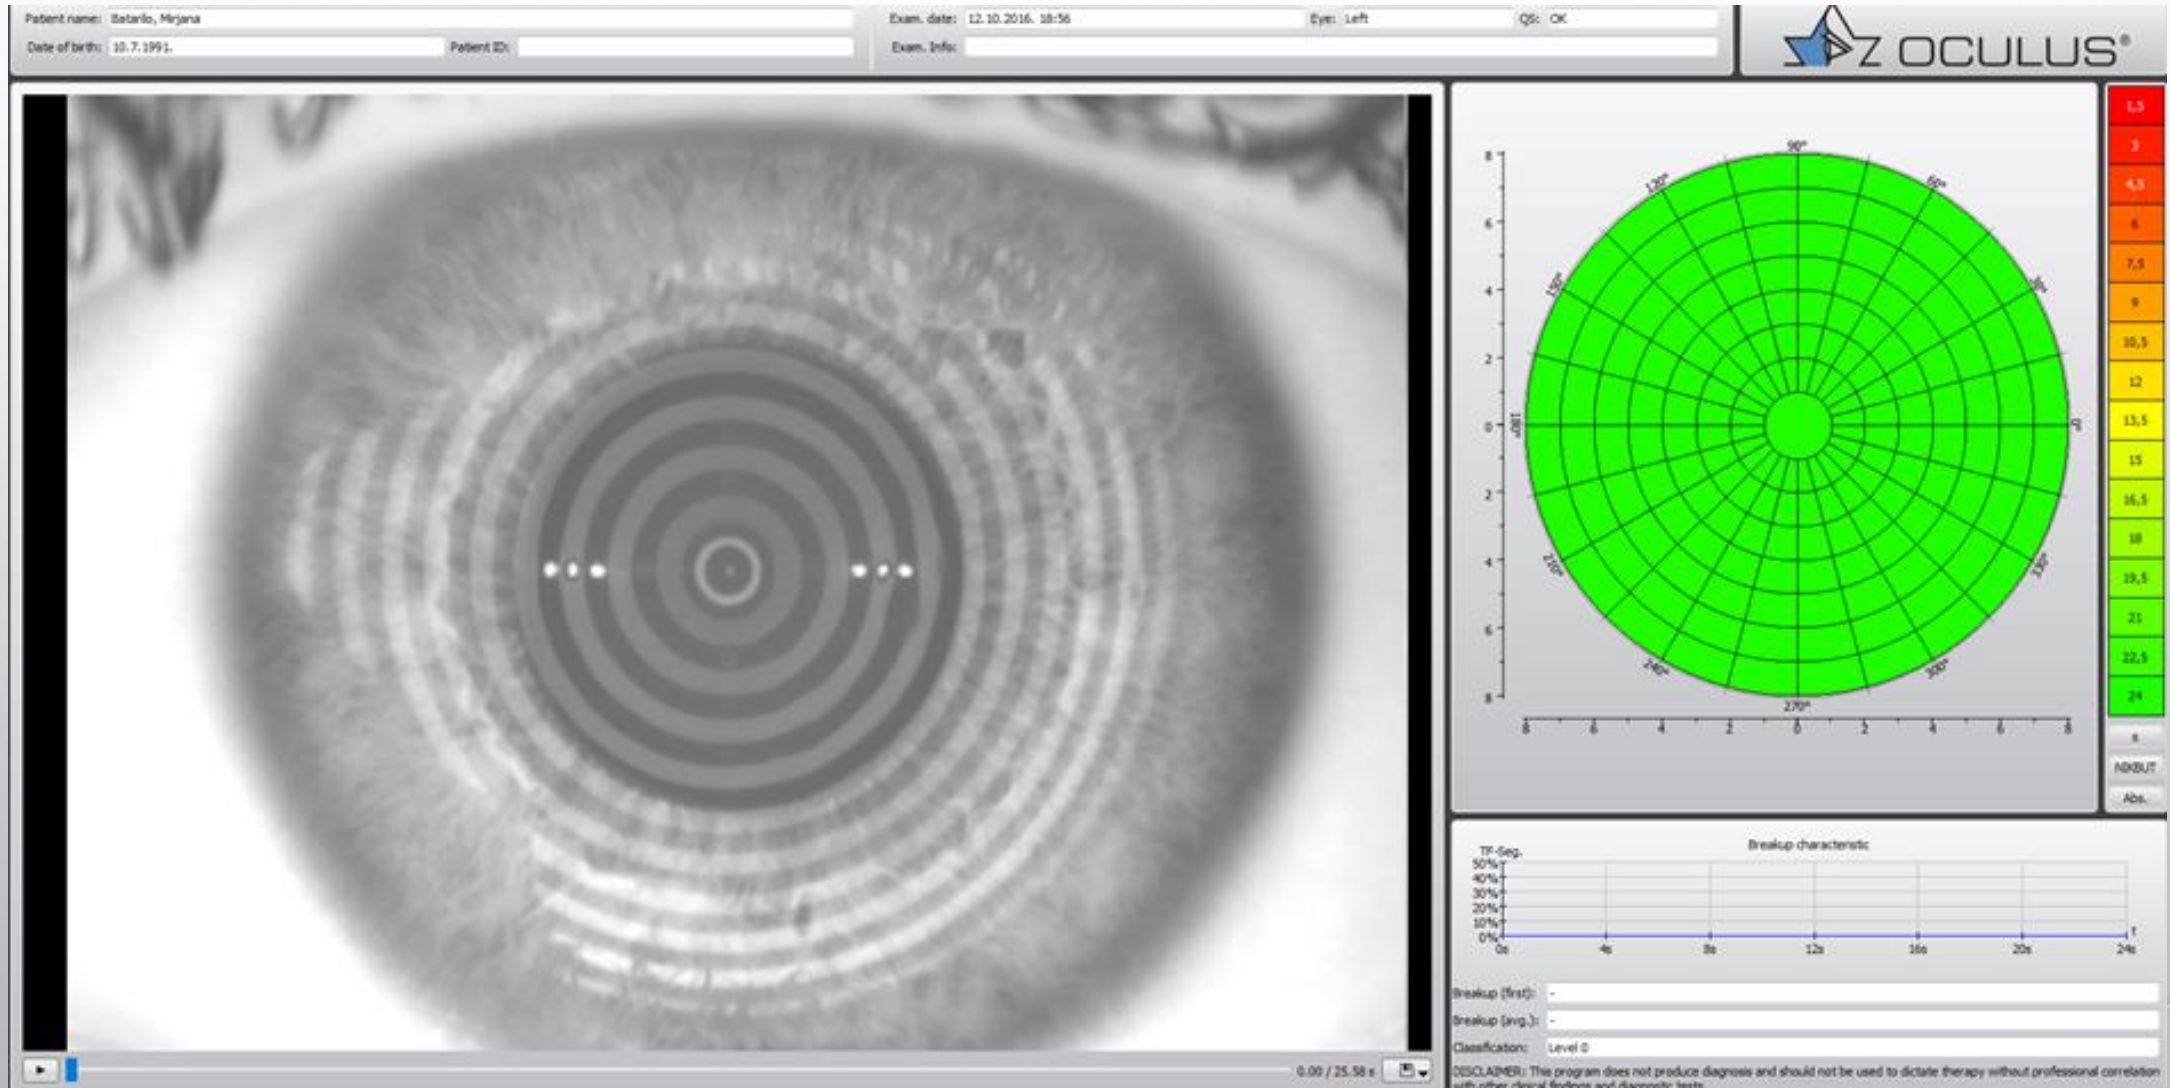


KERATOGRAM


VIRTUALNO FITANJE LEČE

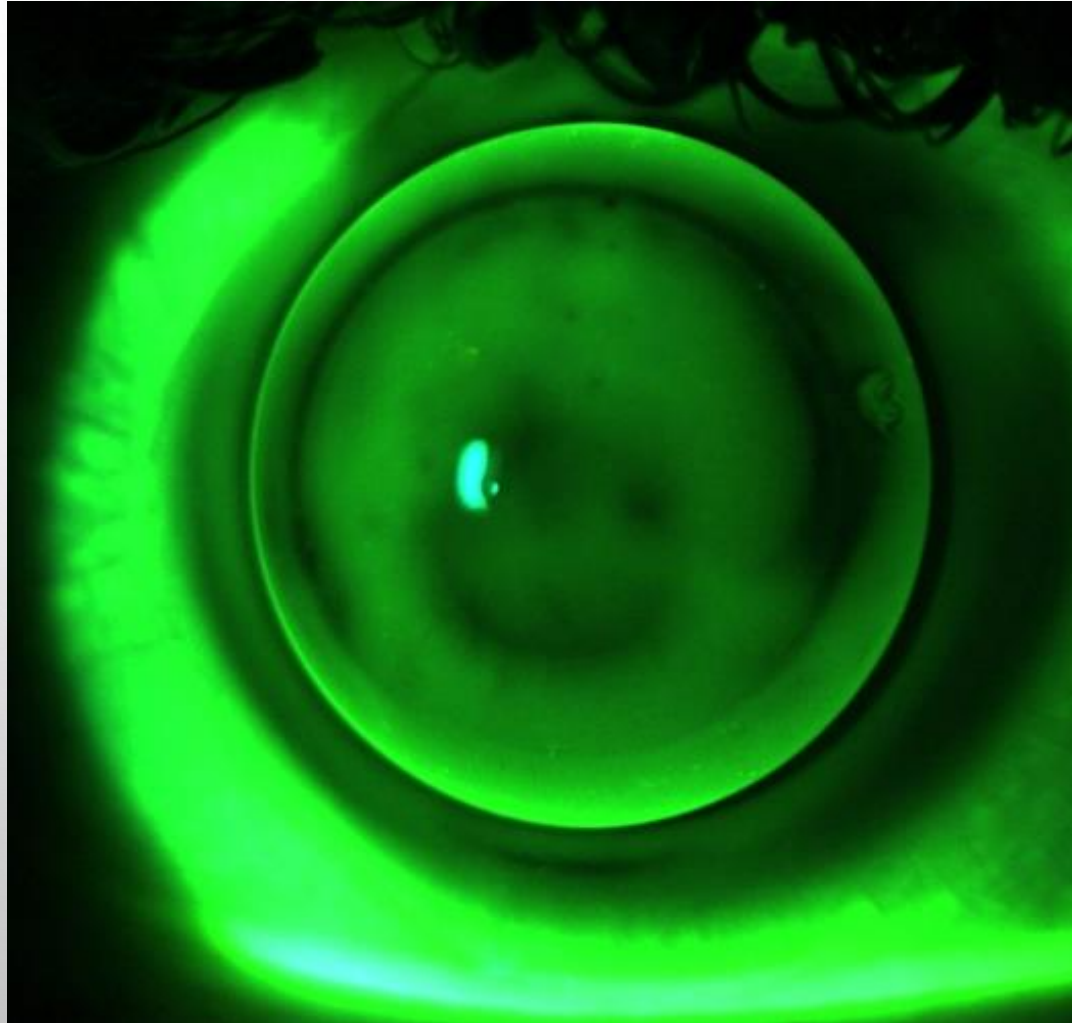


KERATOGRAM

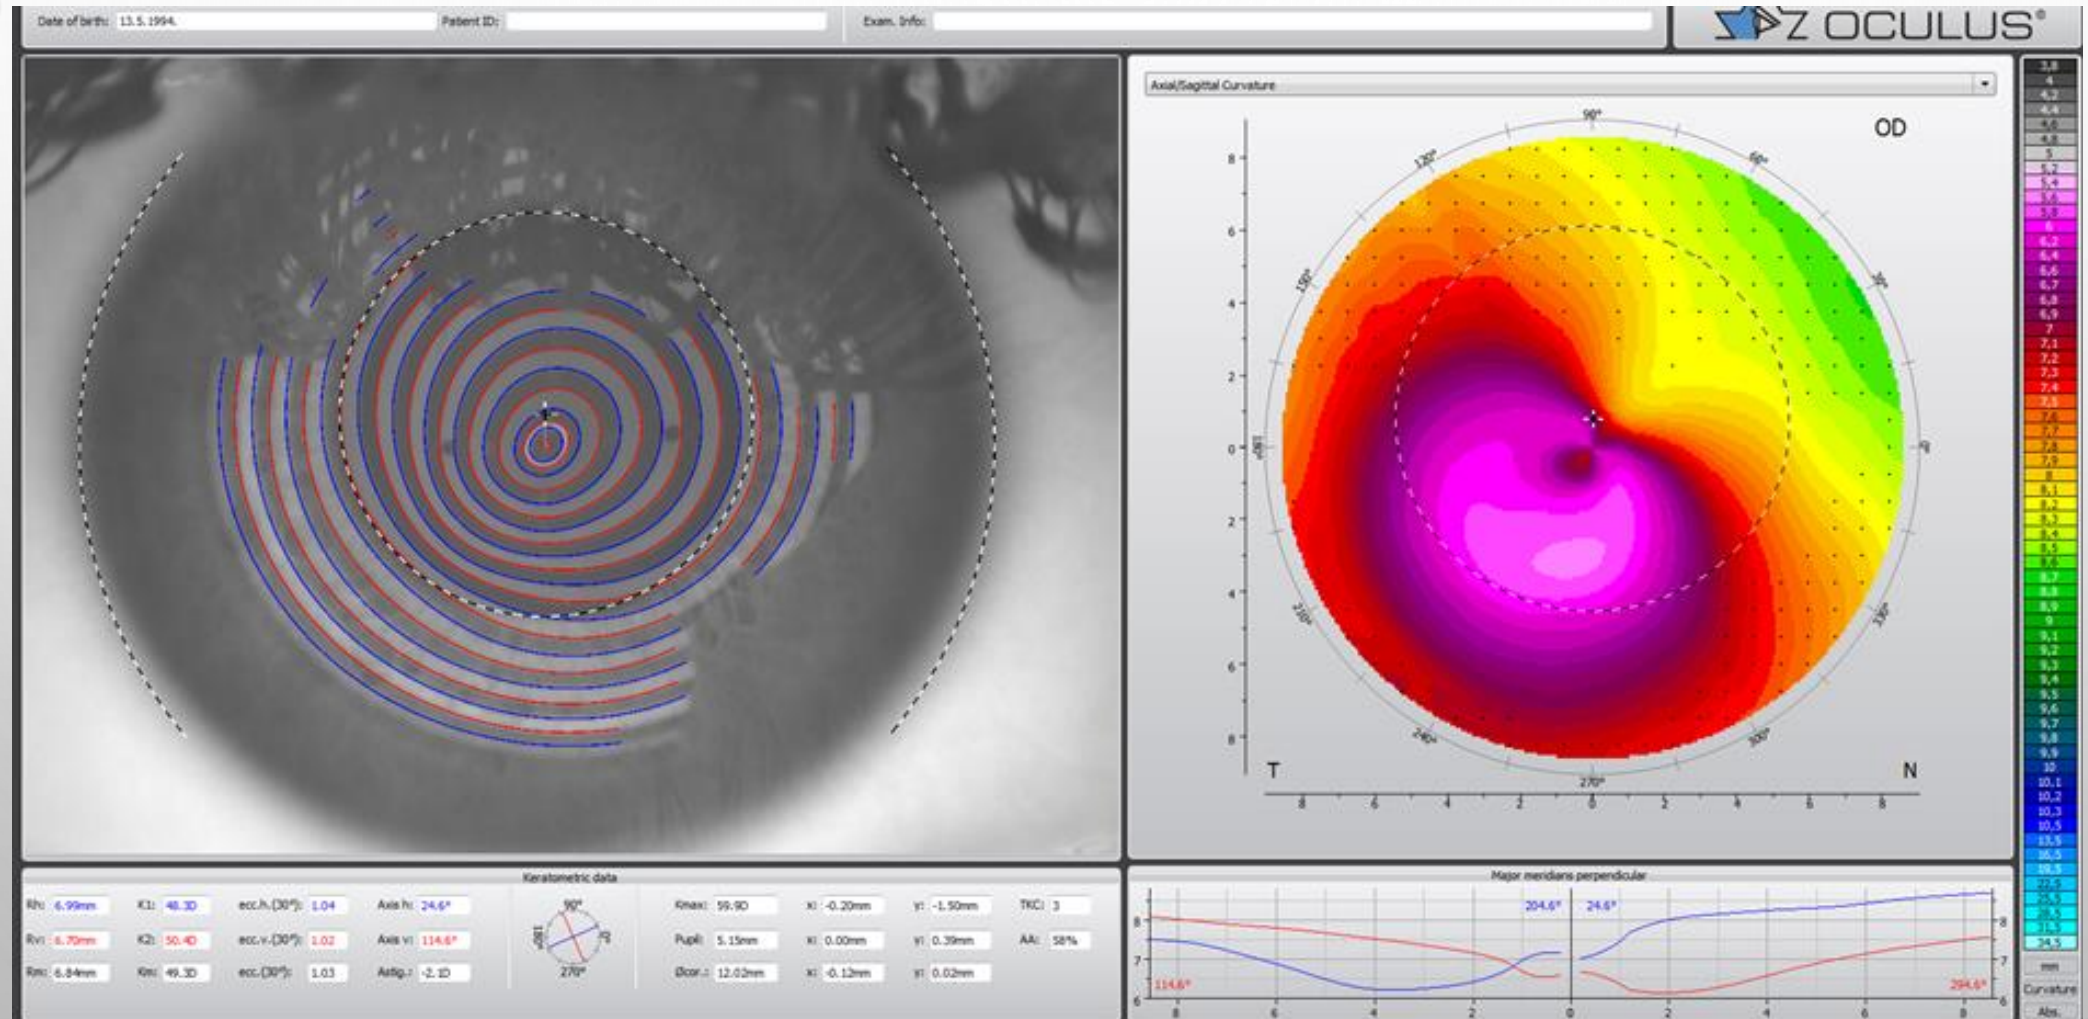

KERATOGRAM

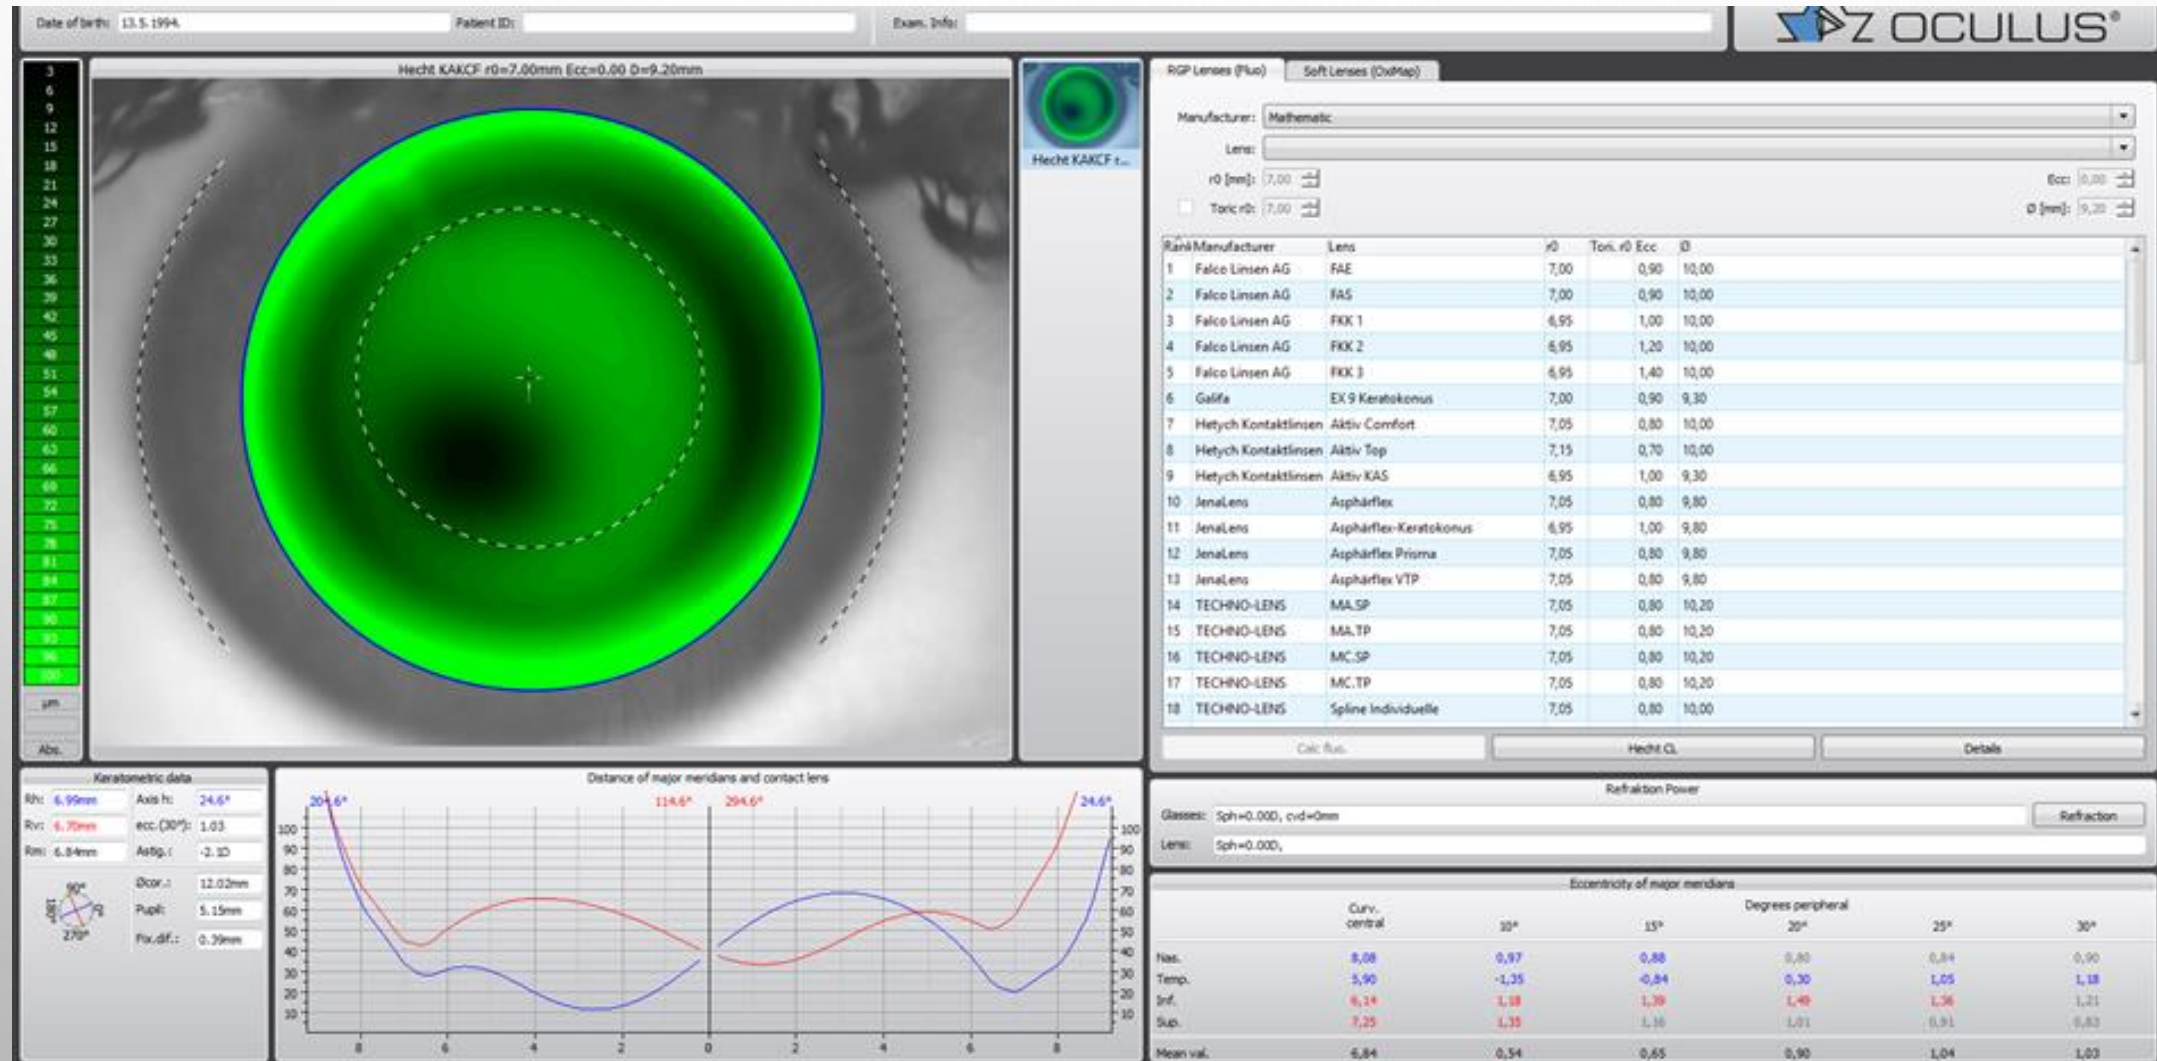

KERATOGRAM

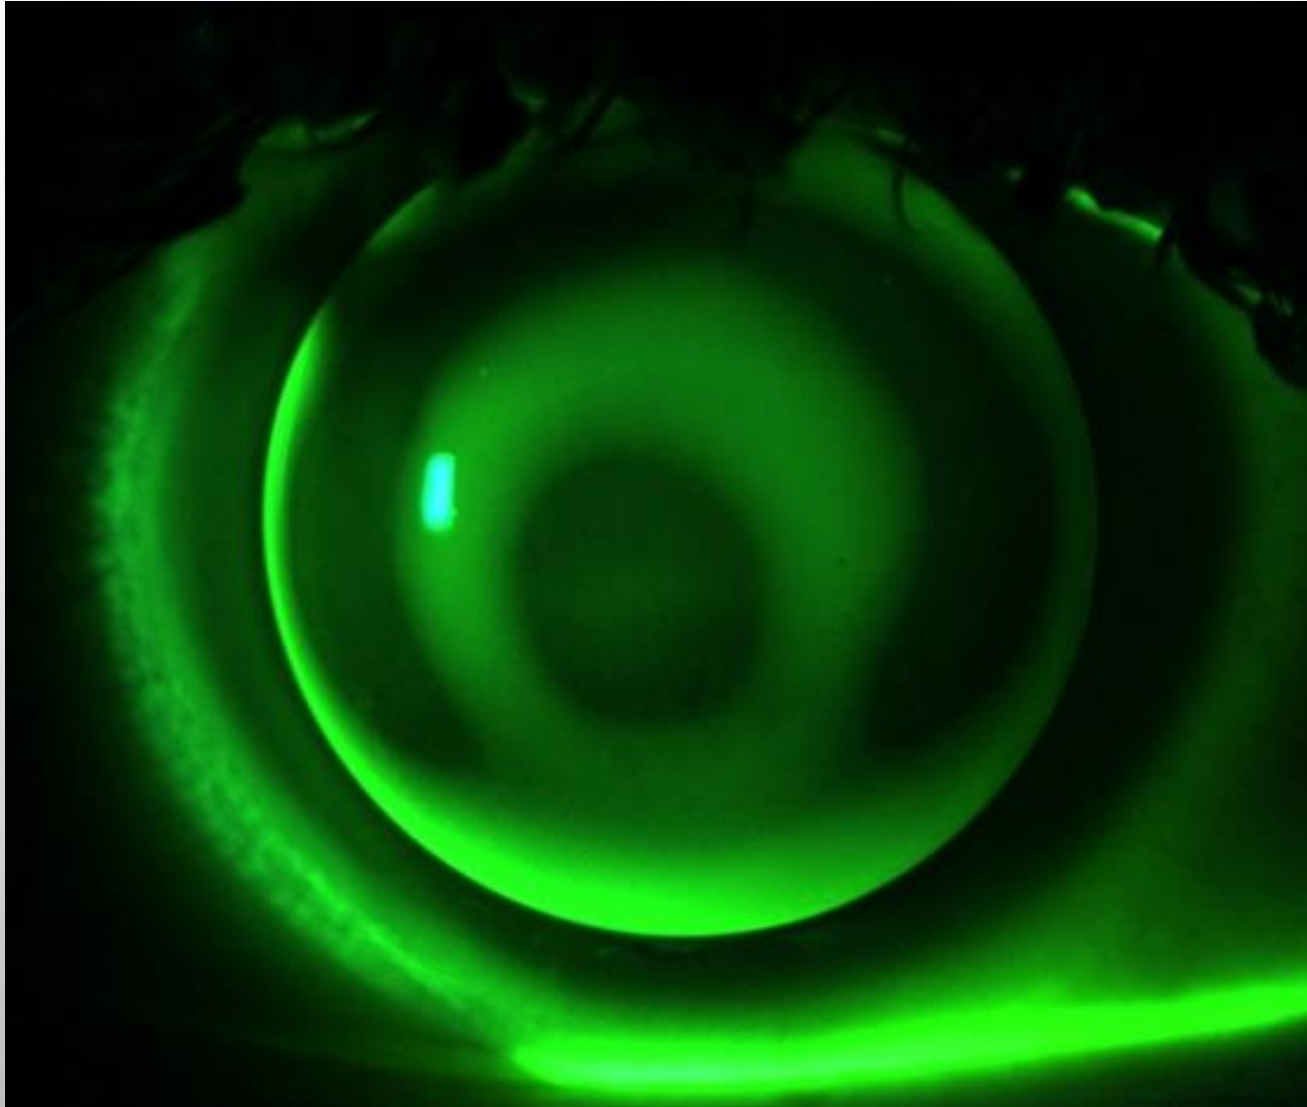


KERATOGRAF


IMAGE CAM




KERATOGRAM

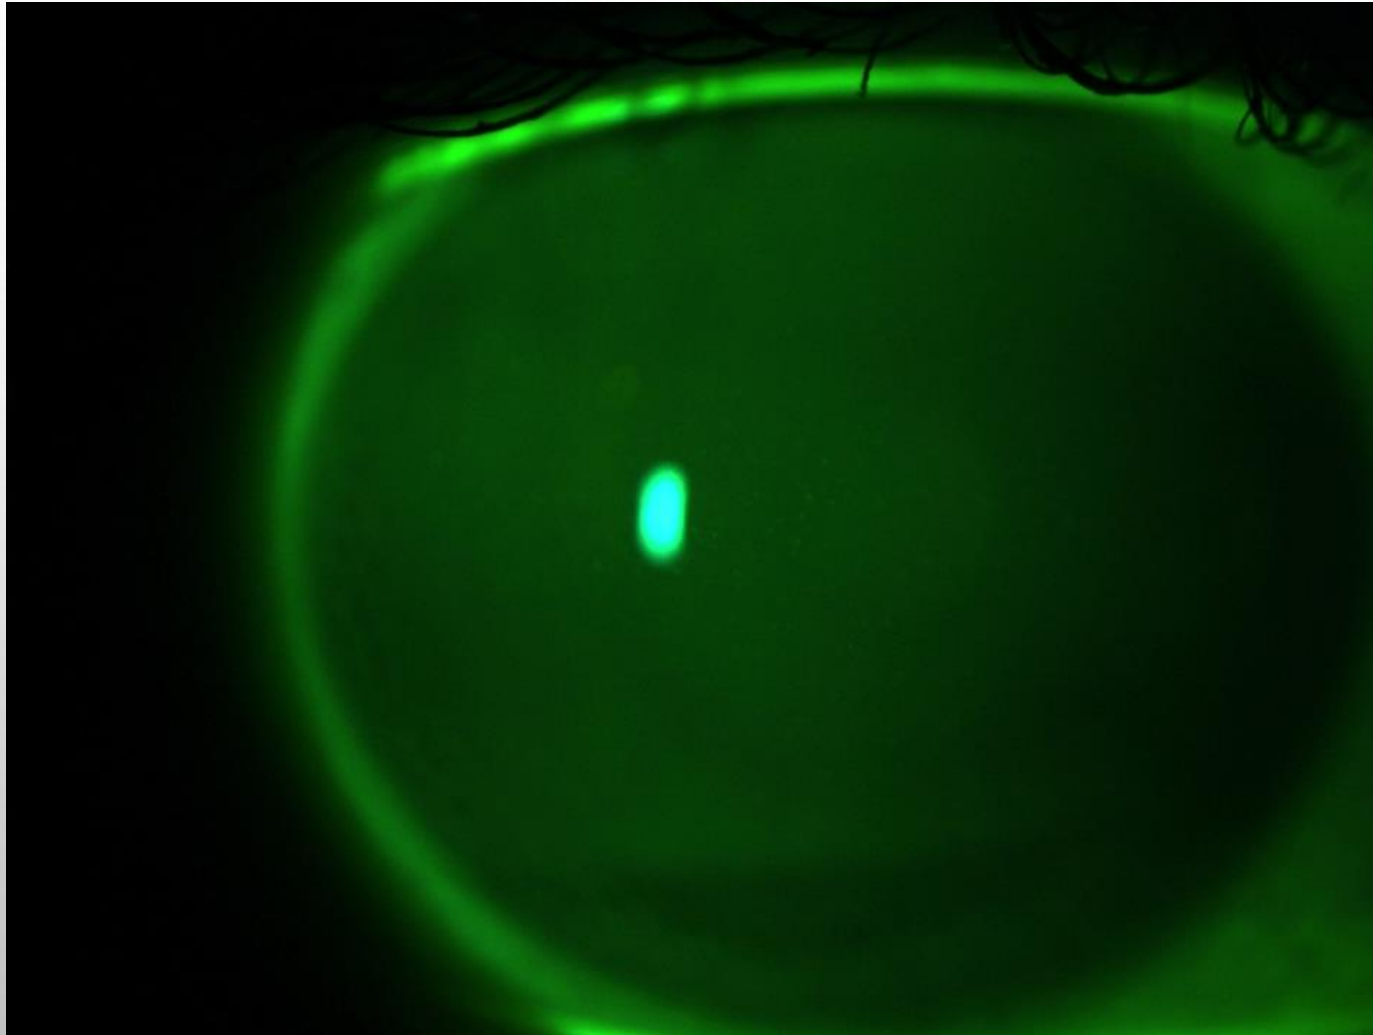


KERATOGRAM

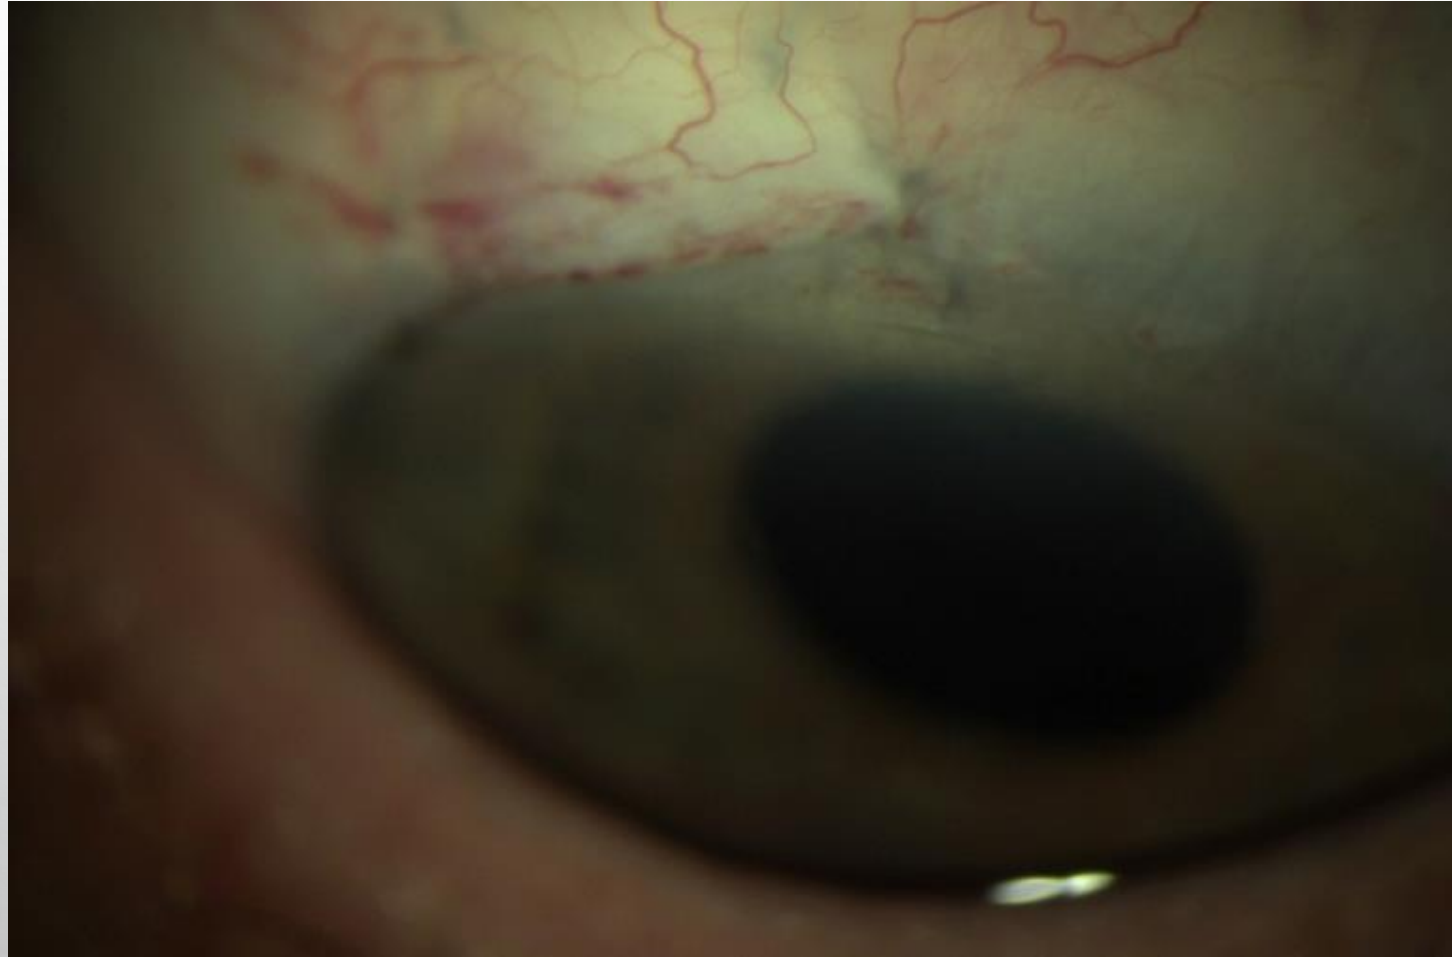


KERATOGRAF

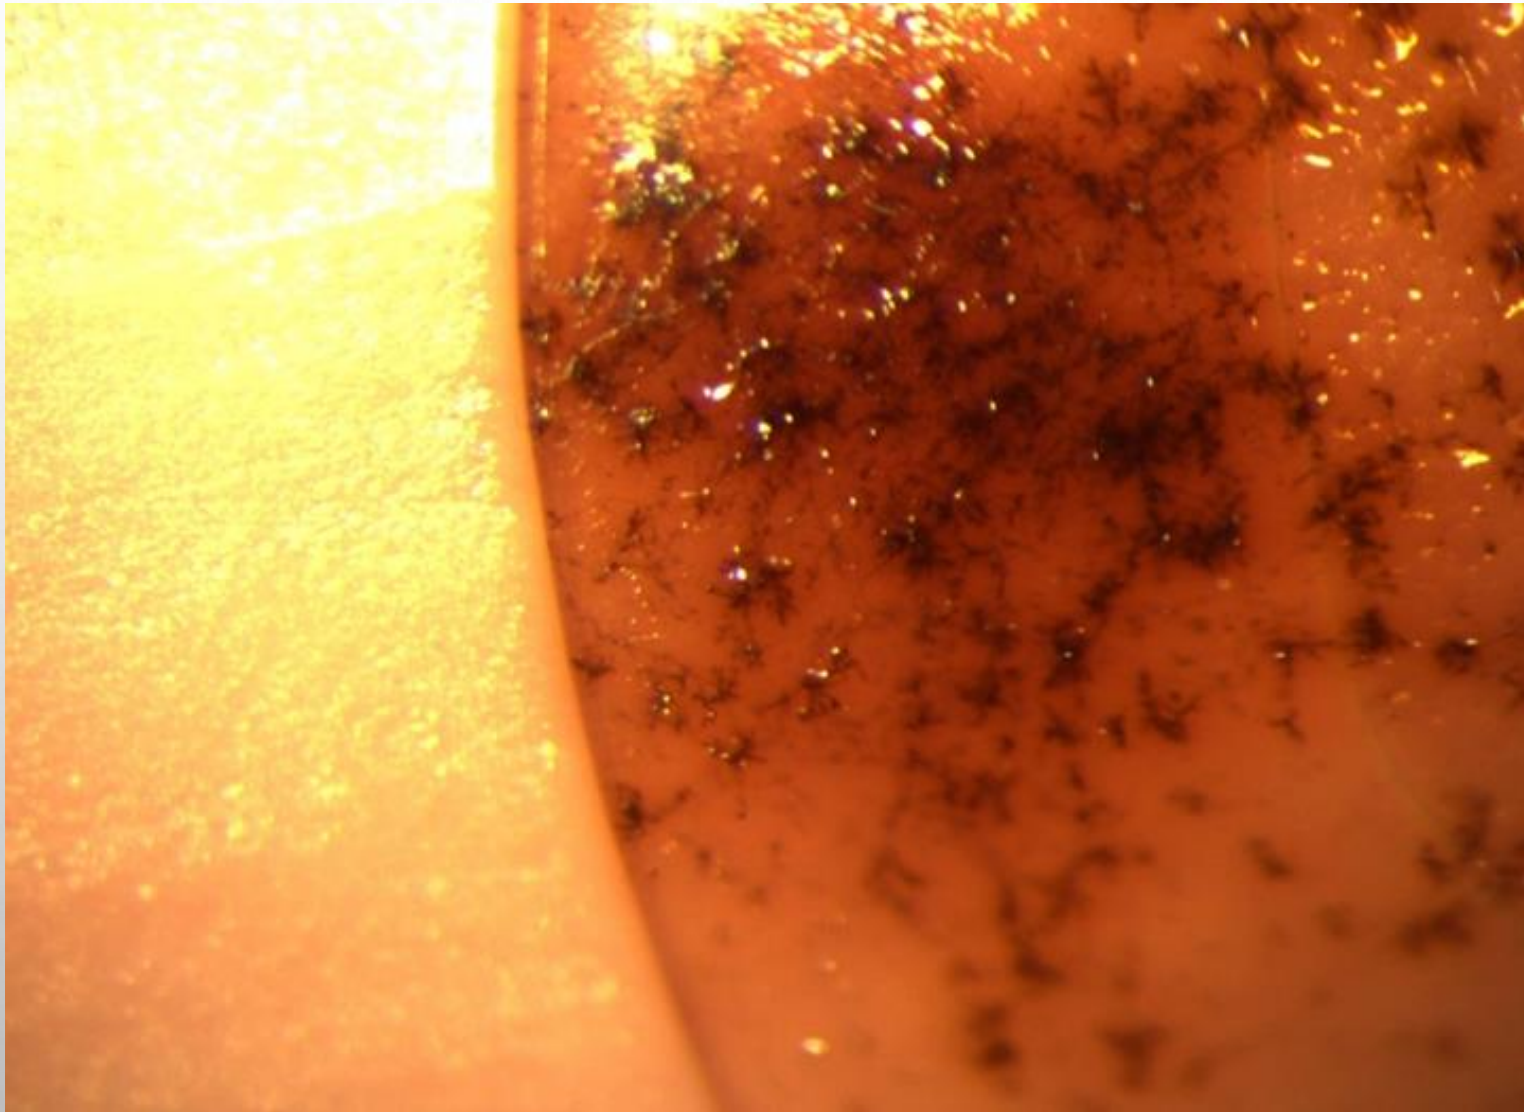

KERATOGRAF

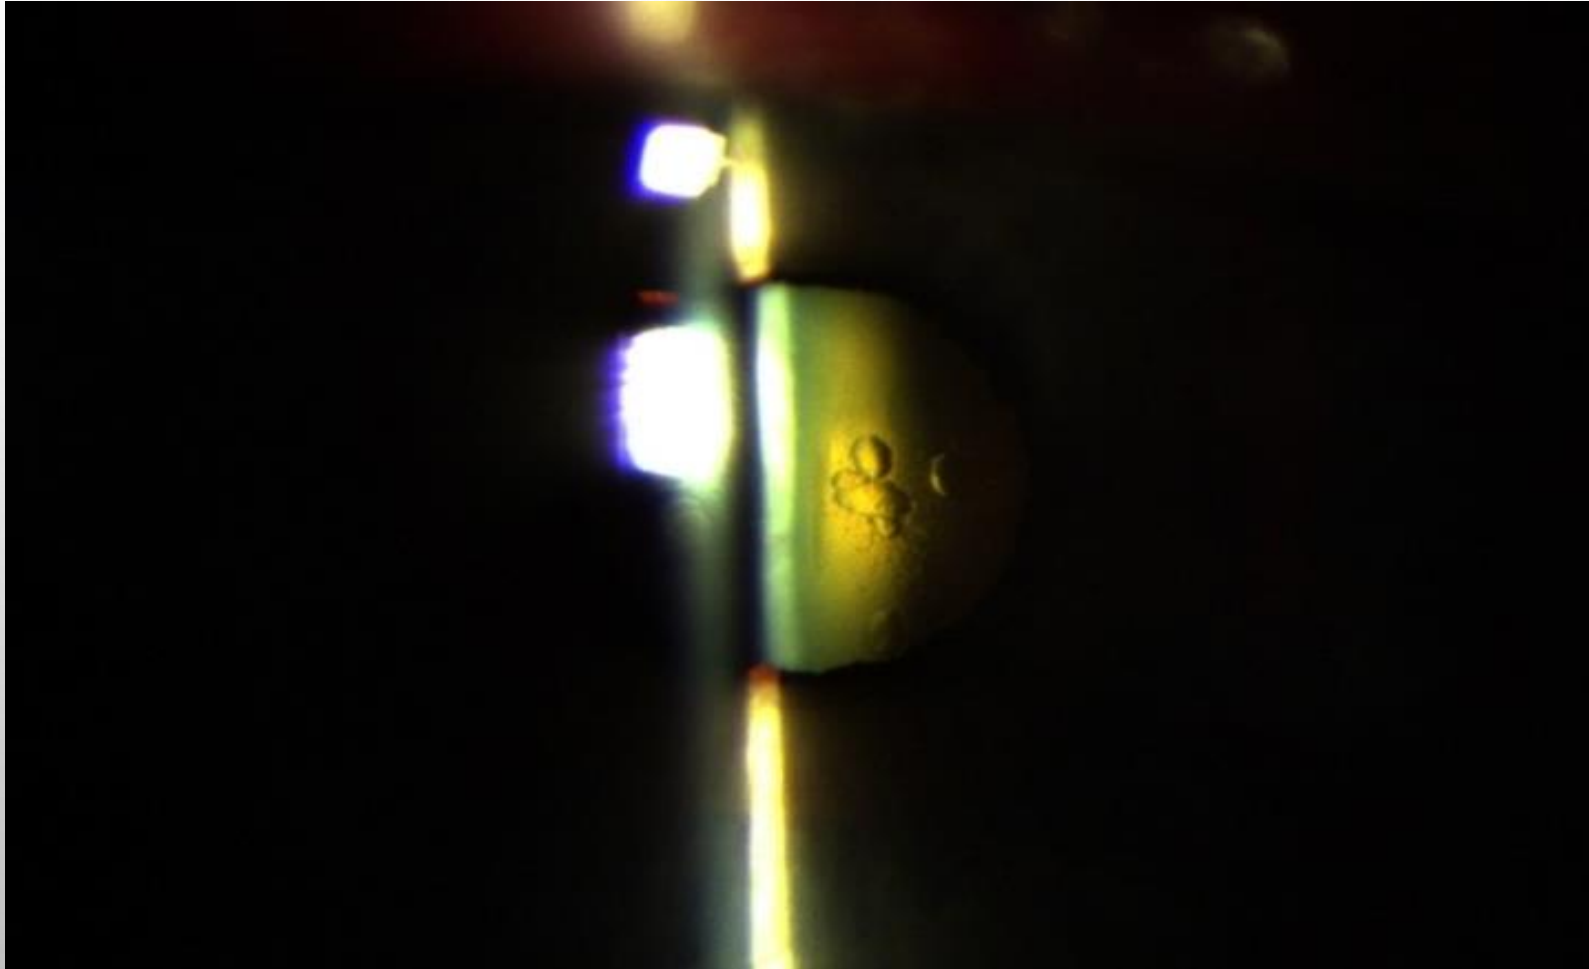

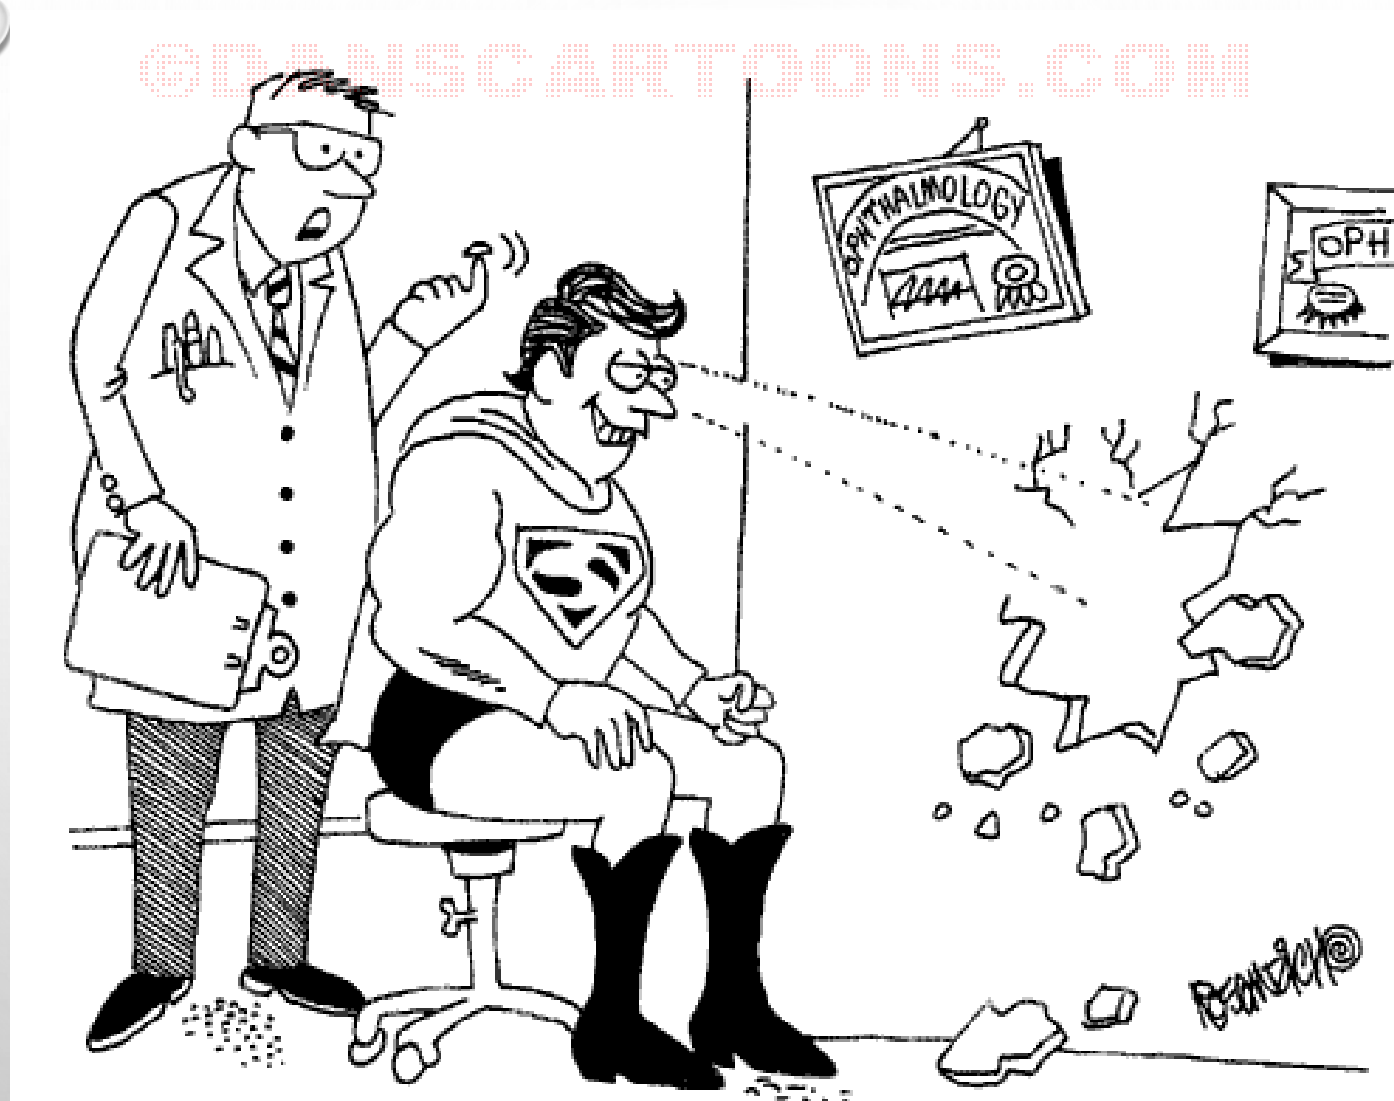

U Vašem slučaju preskočiti ćemo preporuku za kontaktne leće

